

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VW032122\  
 Data File : VW025108.D  
 Acq On : 21 Mar 2022 10:54  
 Operator : SY/MD  
 Sample : N2044-04 20X  
 Misc : 25mL/MSVOA\_V/WATER  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 BFY28

Quant Time: Mar 21 12:13:32 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR031522WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Sat Mar 19 00:53:30 2022  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon           | Response | Conc   | Units    | Dev(Min) |
|-------------------------------|--------|----------------|----------|--------|----------|----------|
| -----                         |        |                |          |        |          |          |
| Internal Standards            |        |                |          |        |          |          |
| 1) 1,4-Difluorobenzene        | 5.613  | 114            | 167795   | 5.000  | ug/L     | 0.00     |
| 28) Chlorobenzene-d5          | 8.850  | 117            | 156284   | 5.000  | ug/L     | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.246 | 152            | 72122    | 5.000  | ug/L     | 0.00     |
|                               |        |                |          |        |          |          |
| System Monitoring Compounds   |        |                |          |        |          |          |
| 4) Vinyl Chloride-d3          | 1.307  | 65             | 55832    | 4.215  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 40 - 130 | Recovery | =      | 84.200%  |          |
| 7) Chloroethane-d5            | 1.568  | 69             | 43628    | 4.497  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 65 - 130 | Recovery | =      | 90.000%  |          |
| 11) 1,1-Dichloroethene-d2     | 2.105  | 63             | 73378    | 3.427  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 60 - 125 | Recovery | =      | 68.600%  |          |
| 20) 2-Butanone-d5             | 3.889  | 46             | 93296    | 58.275 | ug/L     | -0.02    |
| Spiked Amount                 | 50.000 | Range 40 - 130 | Recovery | =      | 116.540% |          |
| 24) Chloroform-d              | 4.343  | 84             | 98938    | 4.503  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 125 | Recovery | =      | 90.000%  |          |
| 26) 1,2-Dichloroethane-d4     | 5.027  | 65             | 43064    | 4.688  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 130 | Recovery | =      | 93.800%  |          |
| 32) Benzene-d6                | 5.043  | 84             | 214945   | 4.741  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 125 | Recovery | =      | 94.800%  |          |
| 36) 1,2-Dichloropropane-d6    | 6.063  | 67             | 63416    | 4.864  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 60 - 140 | Recovery | =      | 97.200%  |          |
| 41) Toluene-d8                | 7.313  | 98             | 187392   | 4.535  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 130 | Recovery | =      | 90.800%  |          |
| 43) trans-1,3-Dichloroprop... | 7.622  | 79             | 19020    | 4.185  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 55 - 130 | Recovery | =      | 83.800%  |          |
| 46) 2-Hexanone-d5             | 8.085  | 63             | 77429    | 49.948 | ug/L     | 0.00     |
| Spiked Amount                 | 50.000 | Range 45 - 130 | Recovery | =      | 99.900%  |          |
| 56) 1,1,2,2-Tetrachloroeth... | 10.214 | 84             | 38360    | 5.002  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 65 - 120 | Recovery | =      | 100.000% |          |
| 66) 1,2-Dichlorobenzene-d4    | 11.622 | 152            | 60925    | 4.990  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 80 - 120 | Recovery | =      | 99.800%  |          |
|                               |        |                |          |        |          |          |
| Target Compounds              |        |                |          |        |          | Qvalue   |
| 16) Methylene chloride        | 2.507  | 84             | 3684     | 0.284  | ug/L     | 92       |
| -----                         |        |                |          |        |          |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV032122\  
Data File : VV025108.D  
Acq On : 21 Mar 2022 10:54  
Operator : SY/MD  
Sample : N2044-04 20X  
Misc : 25mL/MSVOA\_V/WATER  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFY28

Quant Time: Mar 21 12:13:32 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR031522WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Sat Mar 19 00:53:30 2022  
Response via : Initial Calibration

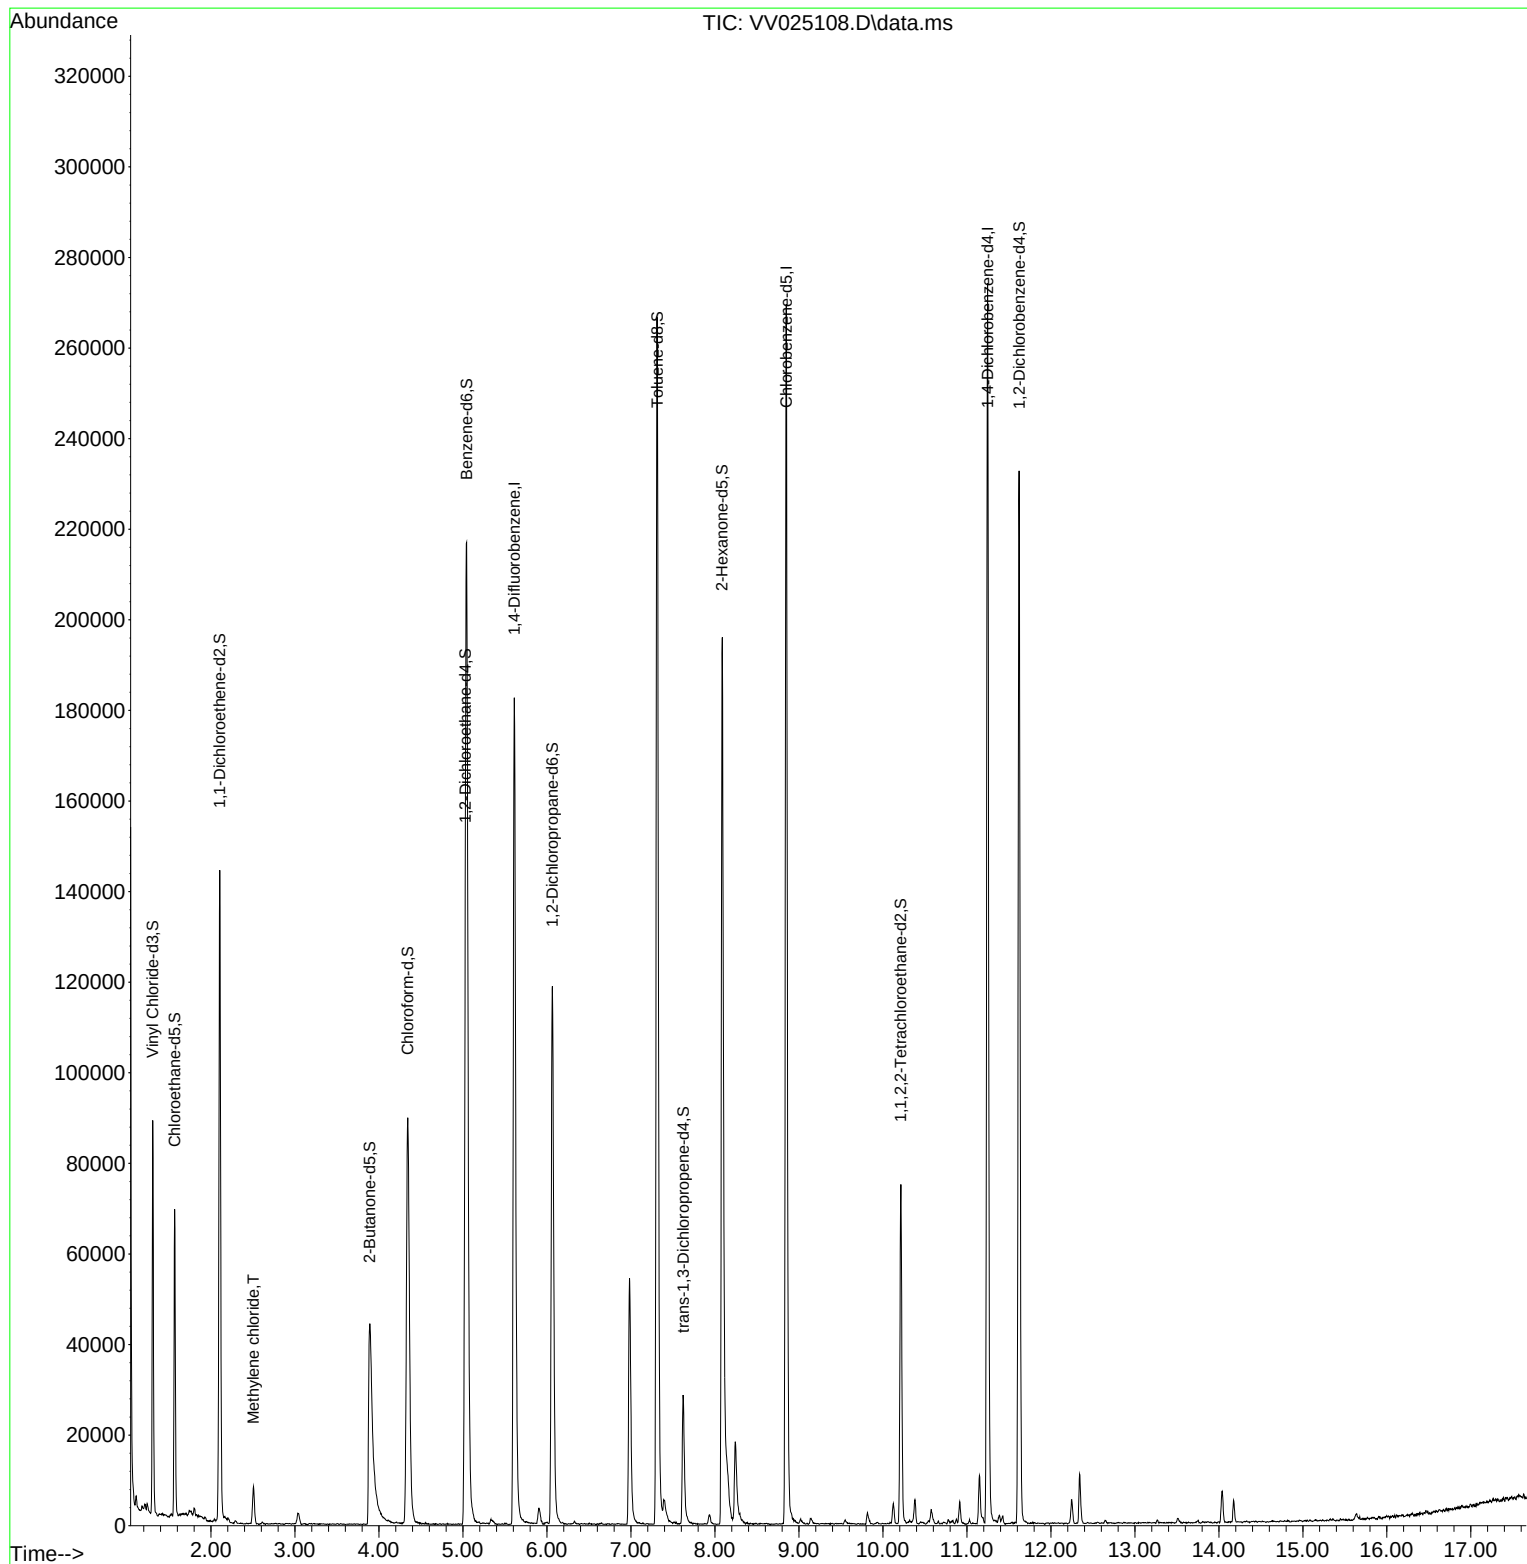

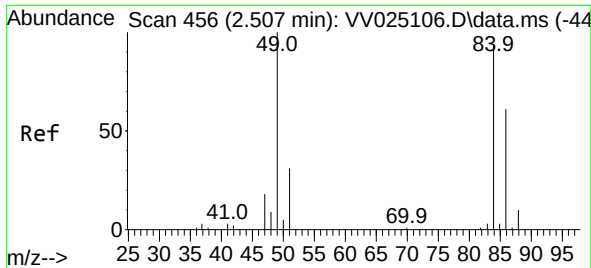

#16  
Methylene chloride  
Concen: 0.284 ug/L  
RT: 2.507 min Scan# 4  
Delta R.T. 0.003 min  
Lab File: VV025108.D  
Acq: 21 Mar 2022 10:54

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFY28

Tgt Ion: 84 Resp: 3684  
Ion Ratio Lower Upper  
84 100  
86 72.5 45.5 84.5  
49 115.2 75.0 139.2

