

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032122\
 Data File : VW025109.D
 Acq On : 21 Mar 2022 11:17
 Operator : SY/MD
 Sample : N2044-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFY27

Quant Time: Mar 21 12:28:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Mar 19 00:53:30 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	161730	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	150963	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	70885	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	54670	4.282	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	85.600%	
7) Chloroethane-d5	1.571	69	44530	4.763	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	95.200%	
11) 1,1-Dichloroethene-d2	2.111	63	71245	3.452	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	69.000%	
20) 2-Butanone-d5	3.892	46	94472	61.222	ug/L	-0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	122.440%	
24) Chloroform-d	4.352	84	99546	4.701	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.000%	
26) 1,2-Dichloroethane-d4	5.037	65	43031	4.860	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	97.200%	
32) Benzene-d6	5.050	84	208762	4.767	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.400%	
36) 1,2-Dichloropropane-d6	6.072	67	60688	4.819	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	96.400%	
41) Toluene-d8	7.317	98	181447	4.546	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	91.000%	
43) trans-1,3-Dichloroprop...	7.625	79	19181	4.369	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	87.400%	
46) 2-Hexanone-d5	8.088	63	78367	52.335	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	104.680%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	37136	5.013	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	100.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	60621	5.052	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	101.000%	
Target Compounds						
13) Acetone	2.182	43	9482	9.188	ug/L	69
47) Tetrachloroethene	7.976	164	819	0.089	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032122\
Data File : VV025109.D
Acq On : 21 Mar 2022 11:17
Operator : SY/MD
Sample : N2044-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFY27

Quant Time: Mar 21 12:28:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Mar 19 00:53:30 2022
Response via : Initial Calibration

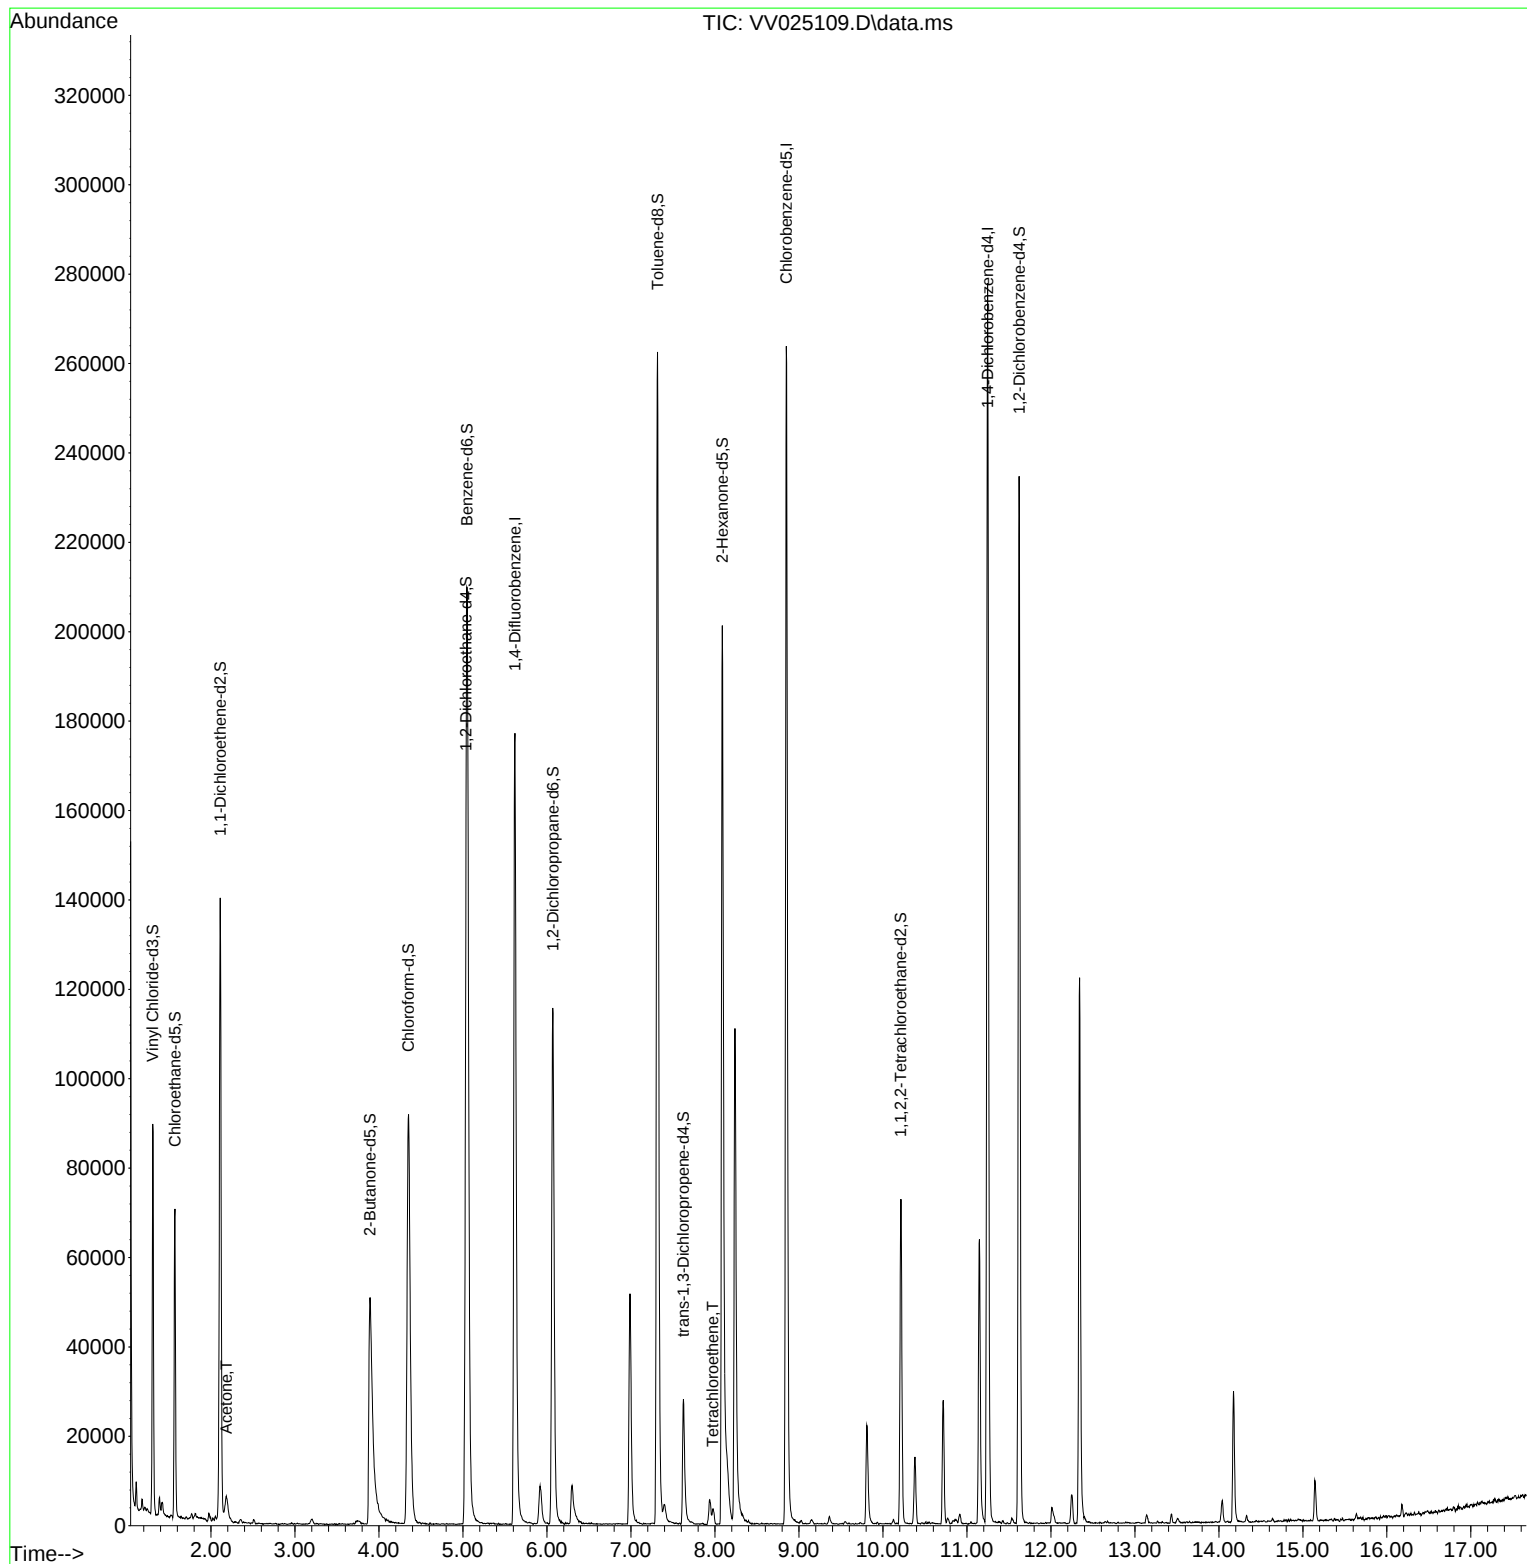

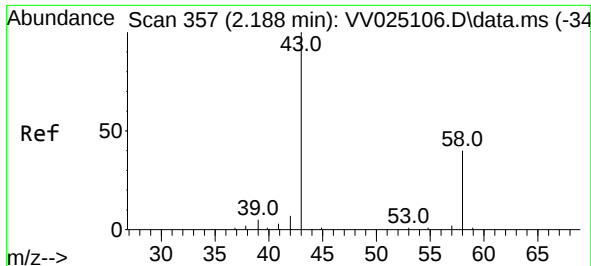

#13

Acetone

Concen: 9.188 ug/L

RT: 2.182 min Scan# 31

Delta R.T. -0.010 min

Lab File: VV025109.D

Acq: 21 Mar 2022 11:17

Instrument :

MSVOA_V

ClientSampleId :





BFY27

Tgt Ion: 43 Resp: 9482

Ion Ratio Lower Upper

43 100

58 43.1 0.0 54.2

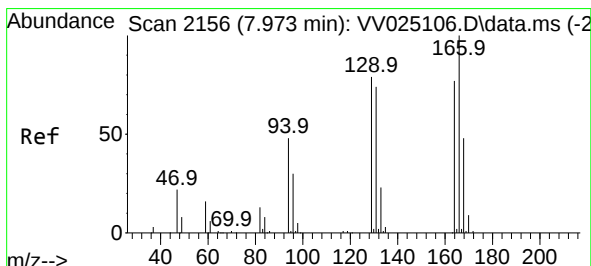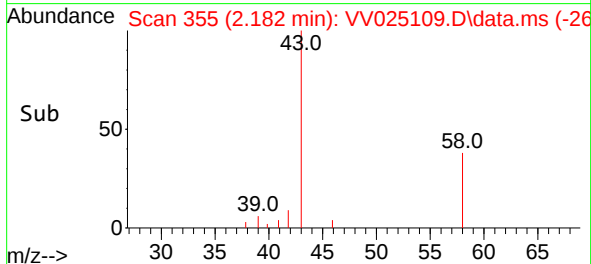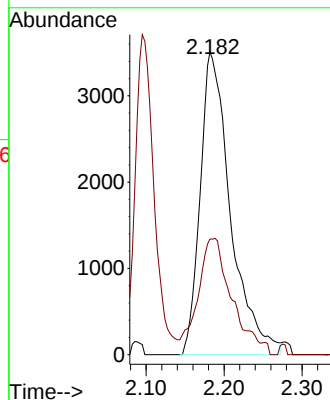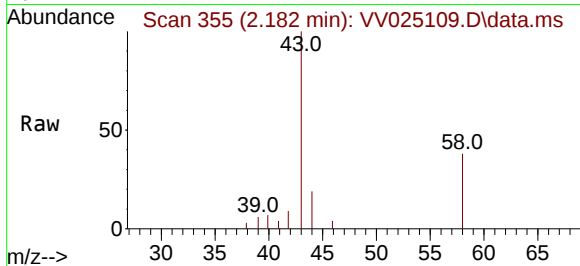

#47

Tetrachloroethene

Concen: 0.089 ug/L

RT: 7.976 min Scan# 2157

Delta R.T. 0.003 min

Lab File: VV025109.D

Acq: 21 Mar 2022 11:17

Tgt Ion:164 Resp: 819

Ion Ratio Lower Upper

164 100

129 84.1 70.3 130.7

131 97.3 69.4 129.0

166 112.5 90.3 167.7

