

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032122\
 Data File : VW025111.D
 Acq On : 21 Mar 2022 12:04
 Operator : SY/MD
 Sample : N2044-02 10X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFY26

Quant Time: Mar 21 12:35:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Mar 19 00:53:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	158580	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	146883	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	68085	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	54579	4.359	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	87.200%	
7) Chloroethane-d5	1.571	69	44031	4.803	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	96.000%	
11) 1,1-Dichloroethene-d2	2.111	63	68995	3.410	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	68.200%	
20) 2-Butanone-d5	3.892	46	90550	59.846	ug/L	-0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	119.700%	
24) Chloroform-d	4.352	84	97665	4.703	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.000%	
26) 1,2-Dichloroethane-d4	5.034	65	42672	4.915	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	98.400%	
32) Benzene-d6	5.050	84	206689	4.851	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.000%	
36) 1,2-Dichloropropane-d6	6.069	67	59790	4.880	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	97.600%	
41) Toluene-d8	7.317	98	180290	4.643	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	92.800%	
43) trans-1,3-Dichloroprop...	7.625	79	18429	4.315	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	86.200%	
46) 2-Hexanone-d5	8.088	63	72917	50.048	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	100.100%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	36580	5.075	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	101.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	58389	5.066	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	101.400%	
Target Compounds						Qvalue
16) Methylene chloride	2.510	84	3265	0.267	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032122\
Data File : VV025111.D
Acq On : 21 Mar 2022 12:04
Operator : SY/MD
Sample : N2044-02 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFY26

Quant Time: Mar 21 12:35:46 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Mar 19 00:53:30 2022
Response via : Initial Calibration

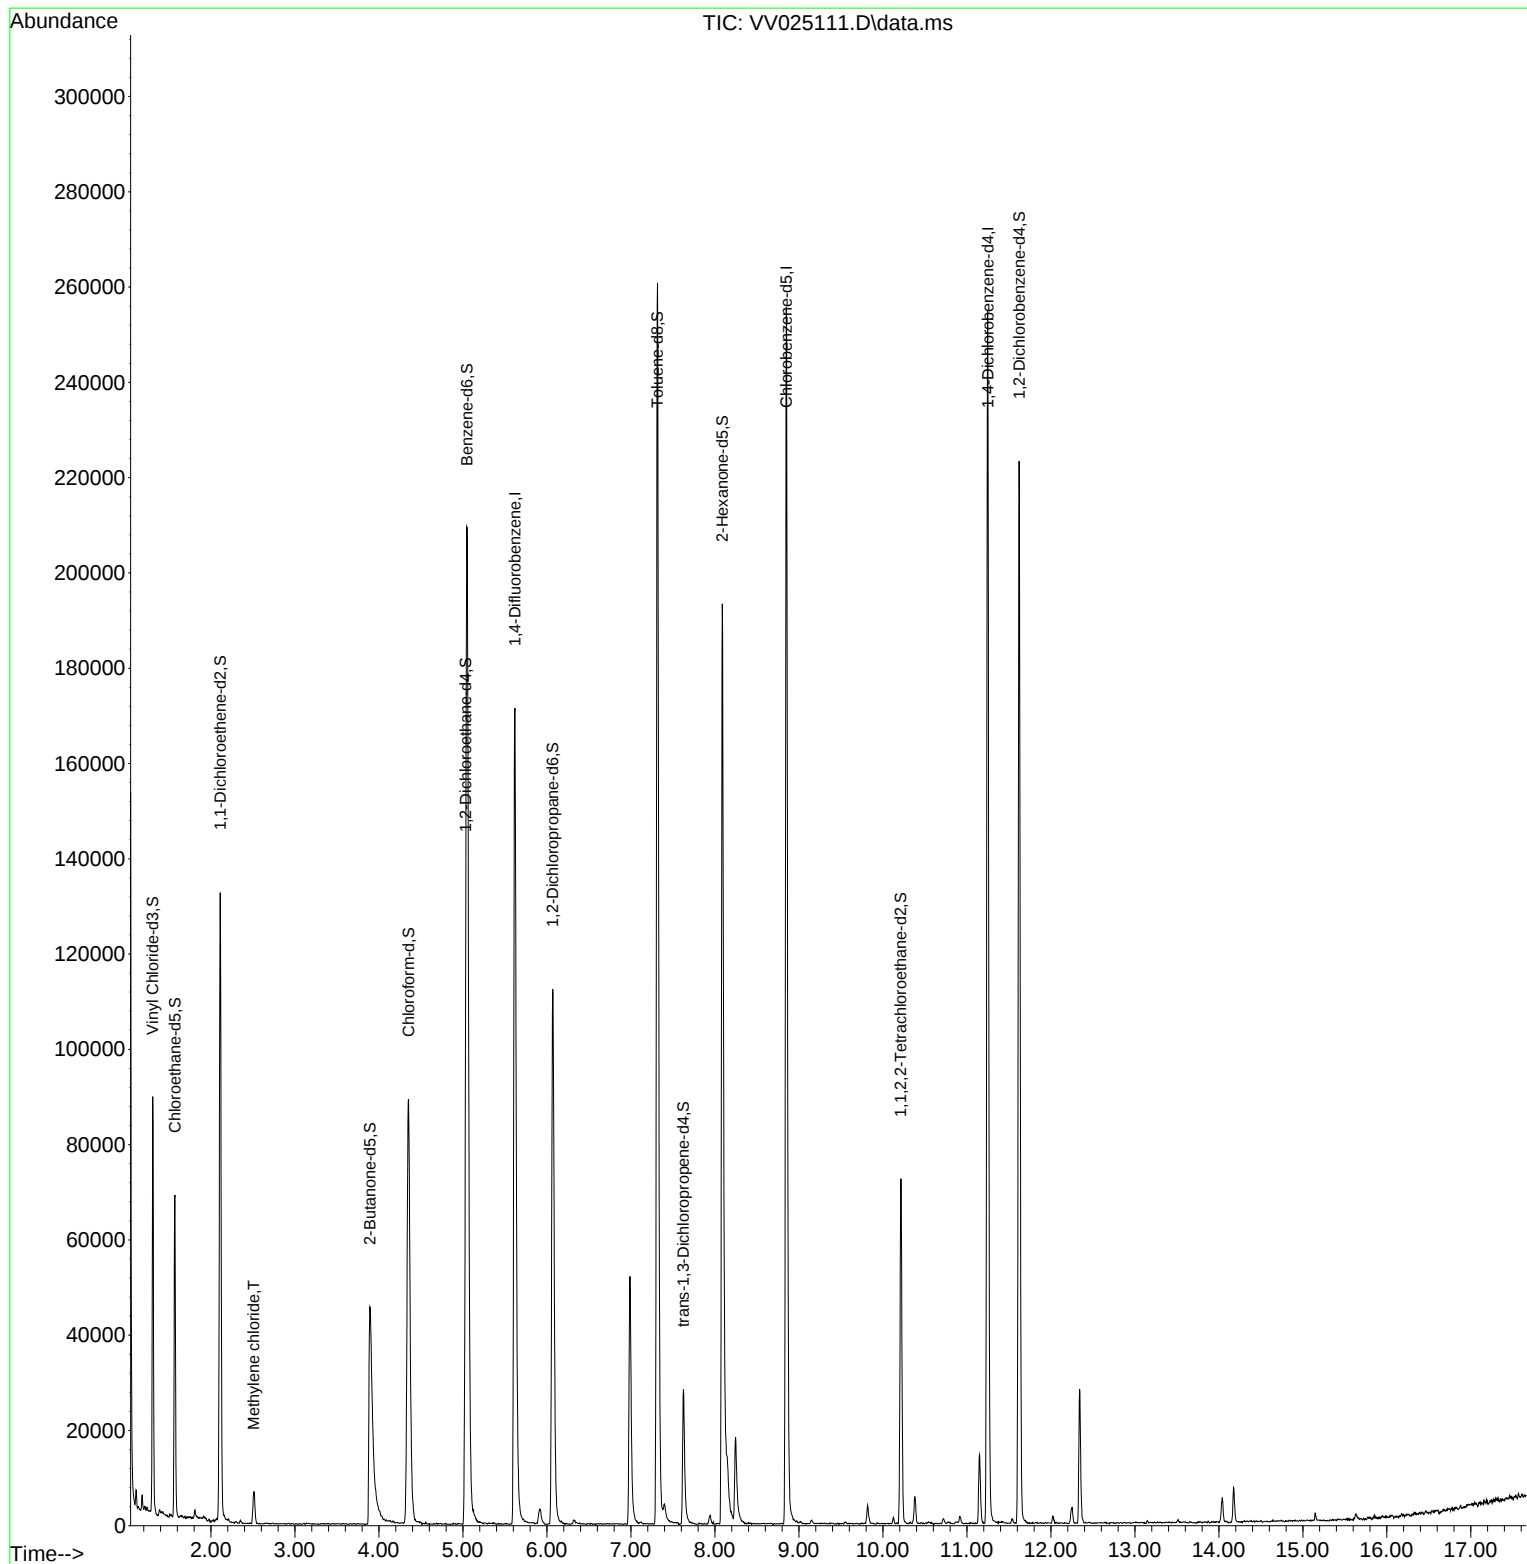

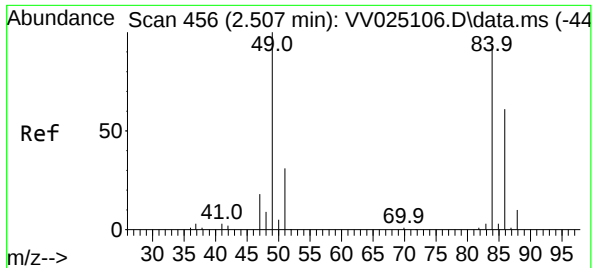

#16
Methylene chloride
Concen: 0.267 ug/L
RT: 2.510 min Scan# 41
Delta R.T. 0.006 min
Lab File: VV025111.D
Acq: 21 Mar 2022 12:04

Instrument :
MSVOA_V
ClientSampleId :
BFY26

Tgt Ion:	84	Resp:	3265
Ion	Ratio	Lower	Upper
84	100		
86	63.9	45.5	84.5
49	102.0	75.0	139.2

