
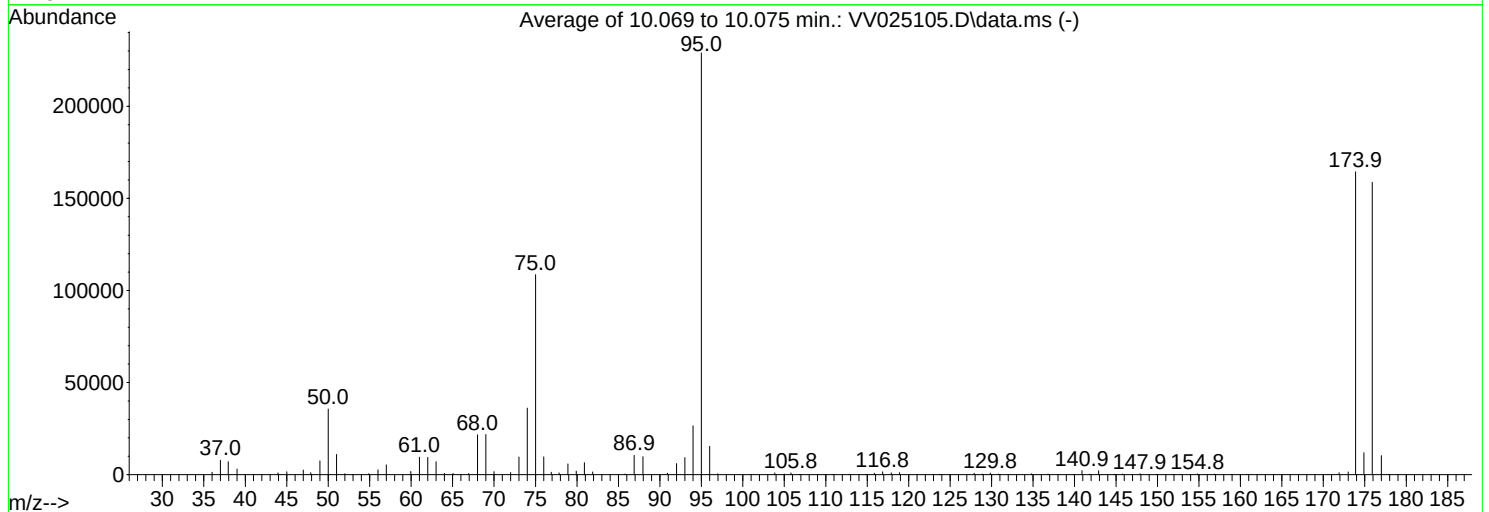


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032122\
 Data File : VV025105.D
 Acq On : 21 Mar 2022 09:03
 Operator : SY/MD
 Sample : BFB283
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB283

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Mar 24 01:12:55 2022

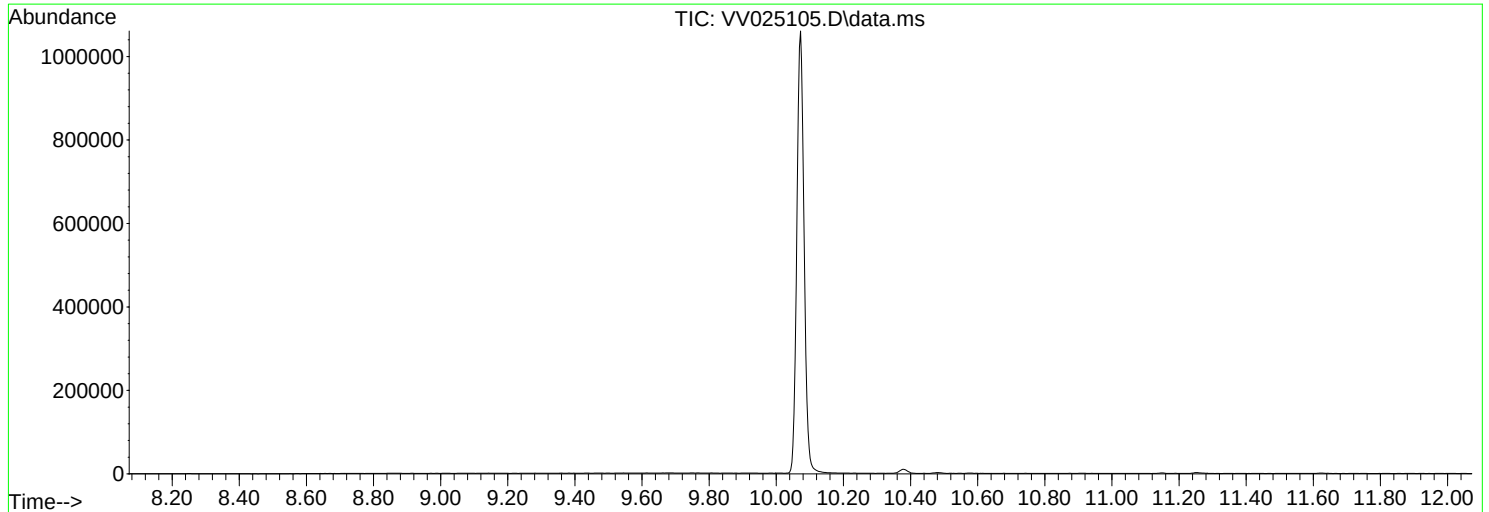

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	35635	PASS
75	95	30	80	47.4	108597	PASS
95	95	100	100	100.0	229013	PASS
96	95	5	9	6.7	15421	PASS
173	174	0.00	2	0.9	1480	PASS
174	95	50	120	71.8	164501	PASS
175	174	5	9	7.2	11891	PASS
176	174	95	105	96.5	158741	PASS
177	176	5	10	6.5	10337	PASS

m/z	Abundance
36.00	940.0
37.90	357.0
39.90	157.0
43.90	301.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283

m/z	Abundance
36.00	2313.0
37.00	8048.0
38.00	7672.0
39.00	3177.0
40.00	246.0
44.00	1222.0
45.00	1596.0
46.00	132.0
47.00	2600.0
47.90	1079.0
49.00	7512.0
50.00	35992.0
51.00	11153.0
52.00	509.0
52.90	122.0
54.90	539.0
56.00	2612.0
57.00	5516.0
58.00	211.0
60.00	1814.0
61.00	9399.0
62.00	9598.0
63.00	7120.0
64.00	656.0
65.10	776.0
67.00	632.0
68.00	21832.0
69.00	22080.0
70.00	1703.0
72.00	1206.0
73.00	9576.0
74.00	36392.0
75.00	110480.0
76.00	9782.0
76.90	1492.0
77.90	1078.0
78.90	5976.0
79.90	1875.0
80.90	6655.0
81.90	1522.0
83.00	174.0
85.80	317.0
86.90	10507.0
88.00	10091.0
90.90	808.0
92.00	6052.0
93.00	9470.0
94.00	26768.0
95.00	228160.0
96.00	15565.0
96.90	457.0
103.90	968.0
105.00	366.0
105.80	1040.0
106.80	193.0
109.90	115.0
110.90	167.0
112.80	243.0
114.90	198.0
115.90	716.0
116.90	1653.0
117.90	897.0
118.90	1157.0
127.90	823.0
128.80	320.0
129.80	782.0
130.90	363.0
134.80	462.0
136.80	284.0
139.80	120.0
140.90	2221.0
141.80	319.0
142.90	2033.0
144.00	121.0
144.80	296.0
145.80	325.0
147.90	565.0
148.90	163.0
149.80	236.0
151.90	154.0
152.80	148.0
153.90	126.0
154.80	435.0
156.90	283.0
159.00	200.0
160.80	237.0
171.90	1065.0
173.00	1523.0
173.90	160768.0
174.90	12031.0
175.90	154624.0
177.00	10200.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283

177.90

320.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283

m/z	Abundance
36.00	2288.0
37.00	8103.0
38.00	7625.0
39.00	3130.0
40.00	266.0
44.00	1314.0
45.00	1618.0
46.00	144.0
47.00	2666.0
47.90	1074.0
49.00	7784.0
50.00	36896.0
51.00	11396.0
52.00	542.0
54.90	586.0
56.00	2666.0
57.00	5512.0
58.00	239.0
59.90	1791.0
61.00	9754.0
62.00	9666.0
63.00	7195.0
64.00	699.0
65.10	701.0
66.90	641.0
68.00	22472.0
69.00	22704.0
70.00	1726.0
72.00	1209.0
73.00	9814.0
74.00	37728.0
75.00	112240.0
76.00	9961.0
76.90	1404.0
77.90	1019.0
78.90	6038.0
79.90	1930.0
80.90	6785.0
81.90	1526.0
83.00	155.0
85.80	351.0
86.90	10861.0
87.90	10048.0
90.90	815.0
92.00	6161.0
93.00	9570.0
94.00	27384.0
95.00	237568.0
96.00	16063.0
97.00	441.0
103.80	992.0
105.00	382.0
105.80	1004.0
106.80	186.0
109.90	127.0
110.90	164.0
112.80	276.0
114.90	195.0
115.90	792.0
116.90	1616.0
117.90	969.0
118.90	1169.0
124.90	109.0
127.90	779.0
128.90	399.0
129.90	885.0
130.90	373.0
134.80	420.0
136.80	328.0
139.80	118.0
140.90	2280.0
141.80	317.0
142.90	2216.0
144.00	118.0
144.80	278.0
145.80	310.0
146.90	155.0
147.90	587.0
148.90	156.0
149.90	199.0
151.90	151.0
152.80	166.0
153.90	147.0
154.90	463.0
156.90	365.0
159.00	216.0
160.80	207.0
170.60	121.0
171.90	1074.0
173.00	1531.0
173.90	170496.0
174.90	12339.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283

175.90164736.0

177.0010676.0

177.90306.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283

m/z	Abundance
36.00	2164.0
37.00	7358.0
38.00	6917.0
39.00	2843.0
40.00	266.0
44.00	1219.0
45.00	1427.0
46.00	142.0
47.00	2398.0
47.90	988.0
49.00	7197.0
50.00	34016.0
51.00	10350.0
52.00	468.0
54.90	544.0
56.00	2530.0
57.00	4961.0
58.00	218.0
59.90	1651.0
61.00	9242.0
62.00	8774.0
63.00	6692.0
64.00	668.0
65.00	639.0
66.90	553.0
68.00	20552.0
69.00	20760.0
70.00	1556.0
72.00	1035.0
73.00	9177.0
74.00	34376.0
75.00	103072.0
76.00	9109.0
76.90	1144.0
77.80	863.0
78.90	5481.0
79.90	1817.0
80.90	6136.0
81.90	1354.0
83.00	116.0
85.80	321.0
86.90	10063.0
87.90	9117.0
90.90	774.0
92.00	5736.0
93.00	8983.0
94.00	25232.0
95.00	221312.0
96.00	14636.0
97.00	381.0
103.80	930.0
105.00	329.0
105.80	864.0
106.80	179.0
109.80	122.0
110.80	155.0
112.80	256.0
114.80	186.0
115.80	816.0
116.80	1385.0
117.90	993.0
118.90	1025.0
123.70	122.0
127.90	682.0
128.90	447.0
129.90	928.0
130.80	338.0
134.80	377.0
136.80	372.0
139.90	111.0
140.90	2103.0
141.80	274.0
142.90	2190.0
144.90	215.0
145.80	320.0
146.90	175.0
147.90	544.0
148.80	125.0
149.90	162.0
151.90	122.0
152.90	174.0
153.90	133.0
154.90	439.0
156.90	377.0
159.00	227.0
160.80	163.0
170.50	105.0
171.90	983.0
173.00	1385.0
173.90	162240.0
174.90	11302.0
175.90	156864.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283

177.0010136.0

177.90262.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283