




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032222\
 Data File : VV025123.D
 Acq On : 22 Mar 2022 13:16
 Operator : SY/MD
 Sample : N2044-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFY31

Manual IntegrationsAPPROVED

Quant Time: Mar 23 01:09:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 23 01:08:13 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 03/23/2022
 Supervised By :Semsettin Yesilyurt 03/23/2022

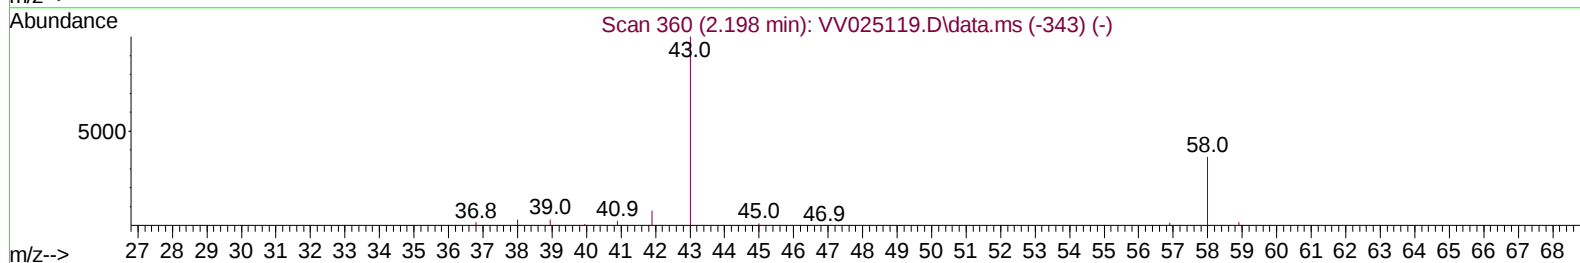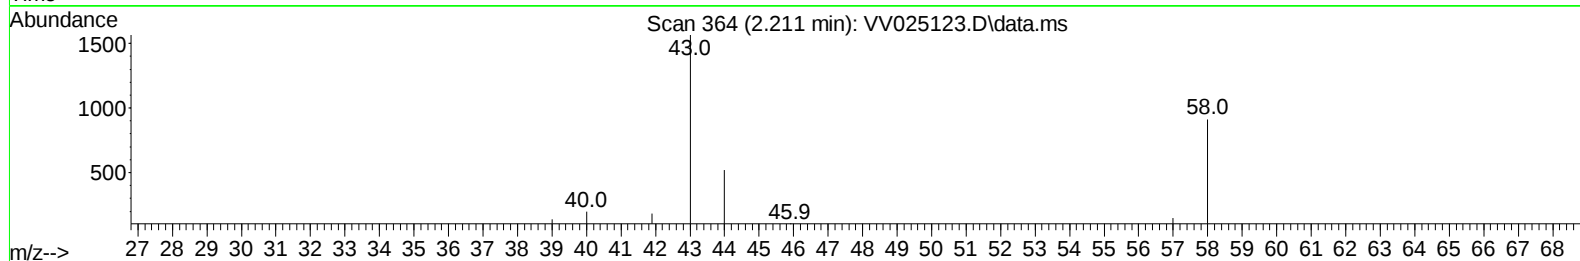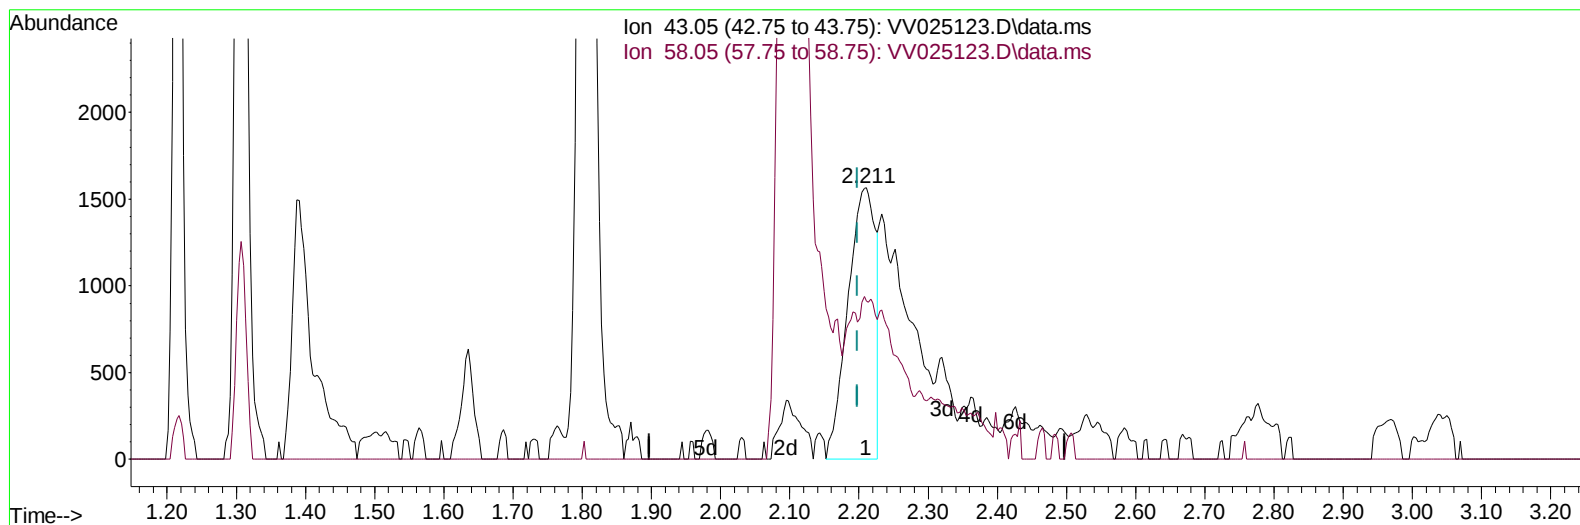

TIC: VV025123.D\data.ms

(13) Acetone (T)

2.211min (+ 0.013) 4.84 ug/L

response 4357

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.10	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032222\
 Data File : VV025123.D
 Acq On : 22 Mar 2022 13:16
 Operator : SY/MD
 Sample : N2044-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFY31

Manual IntegrationsAPPROVED

Quant Time: Mar 23 01:09:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 23 01:08:13 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 03/23/2022
 Supervised By :Semsettin Yesilyurt 03/23/2022

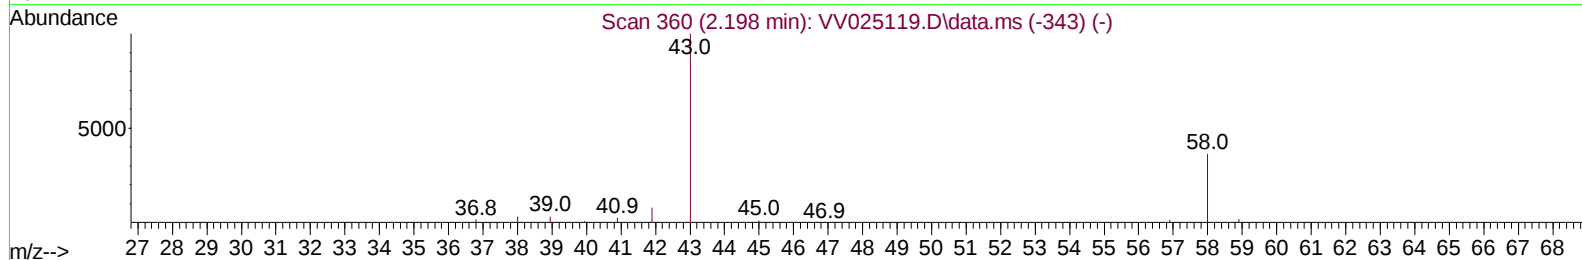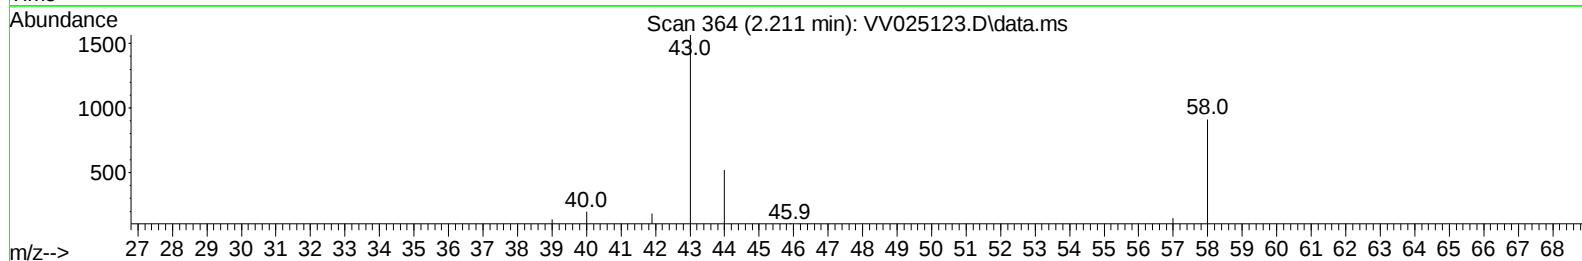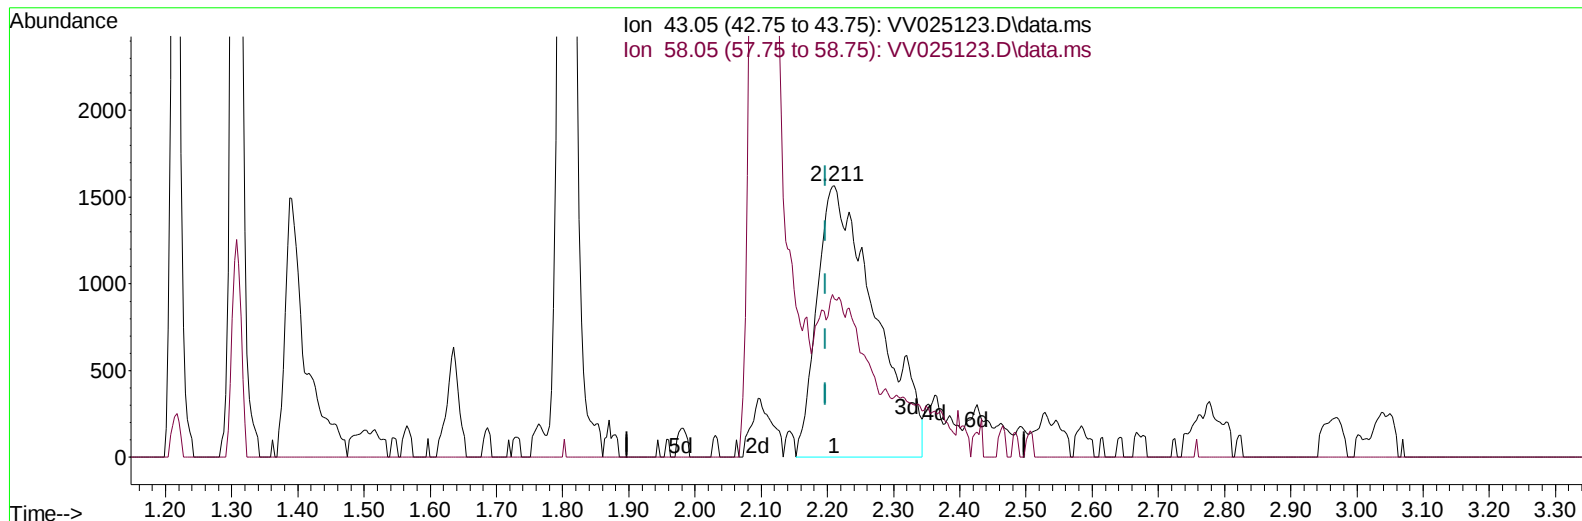

TIC: VV025123.D\data.ms

(13) Acetone (T)

2.211min (+ 0.013) 10.66 ug/L m

response 9601

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.10	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032222\
 Data File : VV025123.D
 Acq On : 22 Mar 2022 13:16
 Operator : SY/MD
 Sample : N2044-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFY31

Manual IntegrationsAPPROVED

Quant Time: Mar 23 01:09:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 23 01:08:13 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 03/23/2022
 Supervised By :Semsettin Yesilyurt 03/23/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	141174	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	130456	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	65201	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	41036	3.682	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	73.600%	
7) Chloroethane-d5	1.568	69	35056	4.295	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	86.000%	
11) 1,1-Dichloroethene-d2	2.108	63	56114	3.115	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	62.400%	
20) 2-Butanone-d5	3.924	46	59324	44.043	ug/L	0.02
Spiked Amount 50.000	Range 40	- 130	Recovery	=	88.080%	
24) Chloroform-d	4.352	84	82444	4.460	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	89.200%	
26) 1,2-Dichloroethane-d4	5.037	65	35246	4.561	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	91.200%	
32) Benzene-d6	5.050	84	168479	4.452	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	89.000%	
36) 1,2-Dichloropropane-d6	6.069	67	52134	4.791	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	95.800%	
41) Toluene-d8	7.317	98	144906	4.201	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	84.000%	
43) trans-1,3-Dichloroprop...	7.625	79	15155	3.995	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	79.800%	
46) 2-Hexanone-d5	8.091	63	62310	48.153	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	96.300%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	31012	4.844	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	96.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	50793	4.602	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	92.000%	
Target Compounds						
					Qvalue	
13) Acetone	2.211	43	9601m	10.658	ug/L	
17) Methyl tert-butyl Ether	2.773	73	2955	0.151	ug/L #	88
19) 1,1-Dichloroethane	3.191	63	1763	0.096	ug/L	99
25) Chloroform	4.384	83	2178	0.114	ug/L	82
33) Benzene	5.101	78	4840	0.114	ug/L	100
63) 1,2,4-Trimethylbenzene	10.915	105	2692	0.068	ug/L #	77

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032222\
Data File : VV025123.D
Acq On : 22 Mar 2022 13:16
Operator : SY/MD
Sample : N2044-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFY31

Manual IntegrationsAPPROVED

Quant Time: Mar 23 01:09:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 23 01:08:13 2022
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 03/23/2022
Supervised By :Semsettin Yesilyurt 03/23/2022

