

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032222\
 Data File : VV025120.D
 Acq On : 22 Mar 2022 11:07
 Operator : SY/MD
 Sample : VV0322WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK321

Quant Time: Mar 23 02:08:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 23 01:08:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	135328	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	126411	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	56850	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	42604	3.988	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	79.800%	
7) Chloroethane-d5	1.568	69	36376	4.650	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	93.000%	
11) 1,1-Dichloroethene-d2	2.108	63	58023	3.360	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	67.200%	
20) 2-Butanone-d5	3.918	46	75347	58.355	ug/L	0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	116.700%	
24) Chloroform-d	4.352	84	84597	4.774	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.400%	
26) 1,2-Dichloroethane-d4	5.034	65	37421	5.051	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	101.000%	
32) Benzene-d6	5.050	84	172519	4.705	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.000%	
36) 1,2-Dichloropropane-d6	6.069	67	53857	5.107	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	102.200%	
41) Toluene-d8	7.317	98	147834	4.423	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	88.400%	
43) trans-1,3-Dichloroprop...	7.625	79	15972	4.345	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	86.800%	
46) 2-Hexanone-d5	8.092	63	66308	52.883	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	105.760%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	32683	5.269	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	105.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	48413	5.030	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	100.600%	
Target Compounds					Qvalue	
25) Chloroform	4.378	83	2090	0.114	ug/L	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032222\
Data File : VV025120.D
Acq On : 22 Mar 2022 11:07
Operator : SY/MD
Sample : VV0322WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK321

Quant Time: Mar 23 02:08:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 23 01:08:13 2022
Response via : Initial Calibration

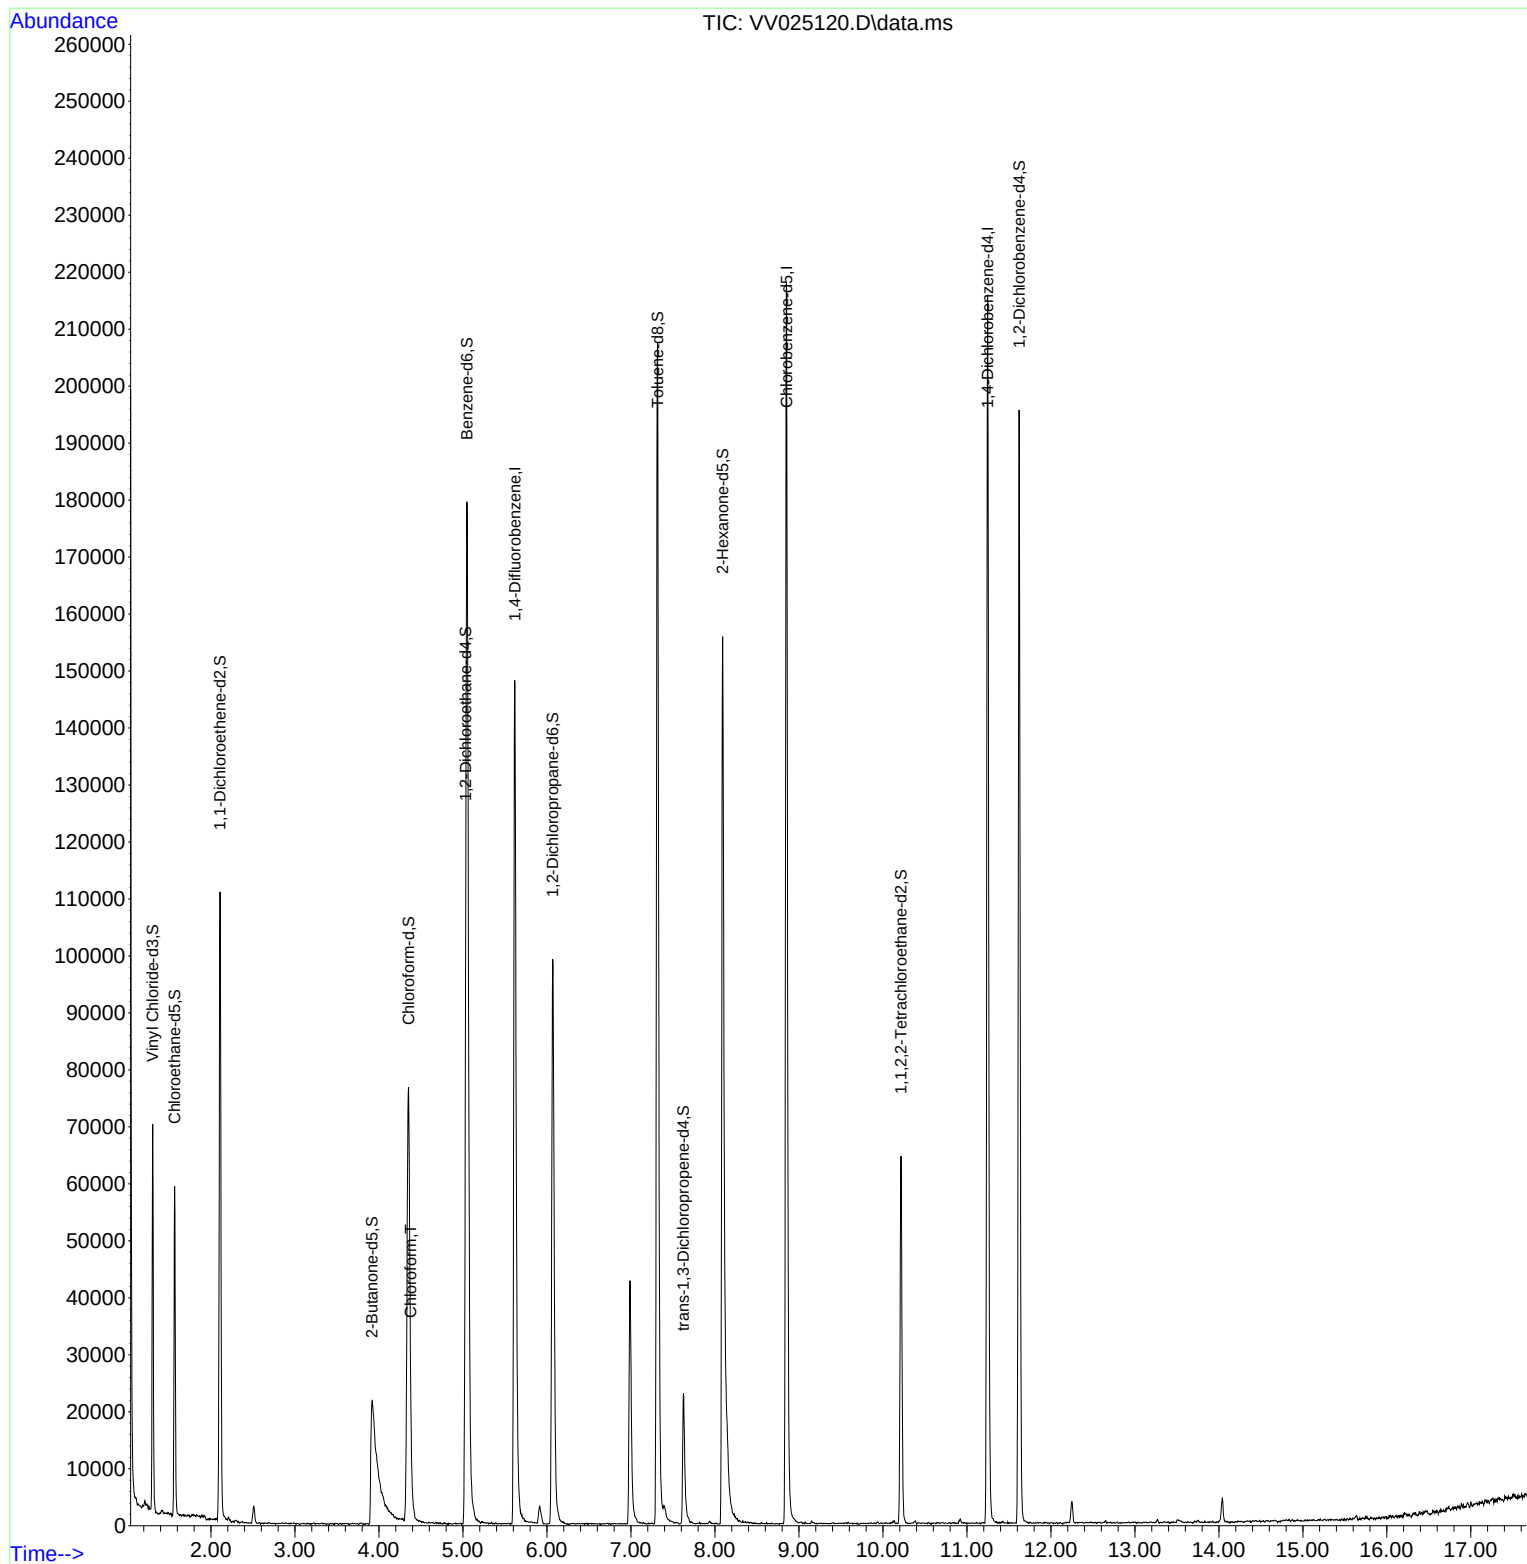

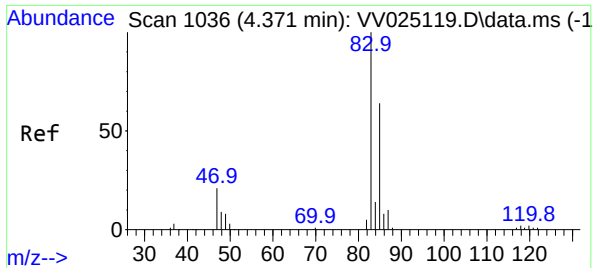

#25
 Chloroform
 Concen: 0.114 ug/L
 RT: 4.378 min Scan# 10
 Delta R.T. 0.007 min
 Lab File: VV025120.D
 Acq: 22 Mar 2022 11:07

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK321

Tgt Ion: 83 Resp: 2090
 Ion Ratio Lower Upper
 83 100
 85 79.7 44.5 82.7

