

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032222\
 Data File : VV025120.D
 Acq On : 22 Mar 2022 11:07
 Operator : SY/MD
 Sample : VV0322WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK321

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025120.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	94	rVB	68223	69132	15.58%	1.978%
2	1.568	156	164	175	rBV	57787	63711	14.36%	1.822%
3	2.108	322	332	348	rBV	110247	157047	35.40%	4.492%
4	2.510	448	457	469	rVB3	3006	4965	1.12%	0.142%
5	3.918	884	895	929	rBV2	21718	103753	23.38%	2.968%
6	4.352	1014	1030	1056	rBV2	76068	194520	43.84%	5.564%
7	5.047	1232	1246	1281	rBV2	179319	443680	100.00%	12.692%
8	5.616	1412	1423	1454	rBV	148040	299223	67.44%	8.559%
9	5.912	1506	1515	1529	rVB4	3133	6705	1.51%	0.192%
10	6.069	1551	1564	1591	rBV	99087	204667	46.13%	5.855%
11	6.989	1840	1850	1880	rBV2	42674	81612	18.39%	2.335%
12	7.317	1939	1952	1972	rBV	207229	371113	83.64%	10.616%
13	7.625	2036	2048	2073	rBV	22896	42413	9.56%	1.213%
14	8.092	2183	2193	2234	rBV	155664	338252	76.24%	9.676%
15	8.850	2418	2429	2470	rBV	217680	363724	81.98%	10.405%
16	10.217	2842	2854	2872	rBV	64495	101506	22.88%	2.904%
17	11.246	3163	3174	3193	rBV	215597	336078	75.75%	9.614%
18	11.622	3280	3291	3310	rBV	195408	300679	67.77%	8.601%
19	12.252	3476	3487	3498	rVB	3788	6229	1.40%	0.178%
20	14.040	4033	4043	4057	rVB	4214	6806	1.53%	0.195%




Sum of corrected areas: 3495815

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032222\
Data File : VV025120.D
Acq On : 22 Mar 2022 11:07
Operator : SY/MD
Sample : VV0322WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK321

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

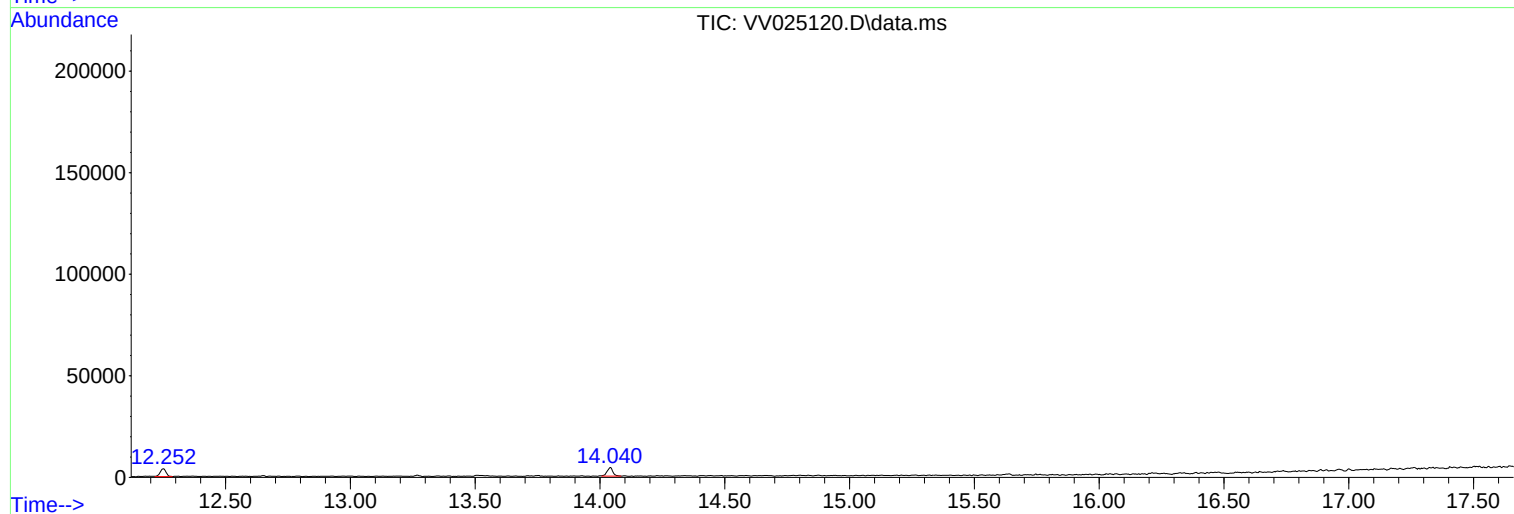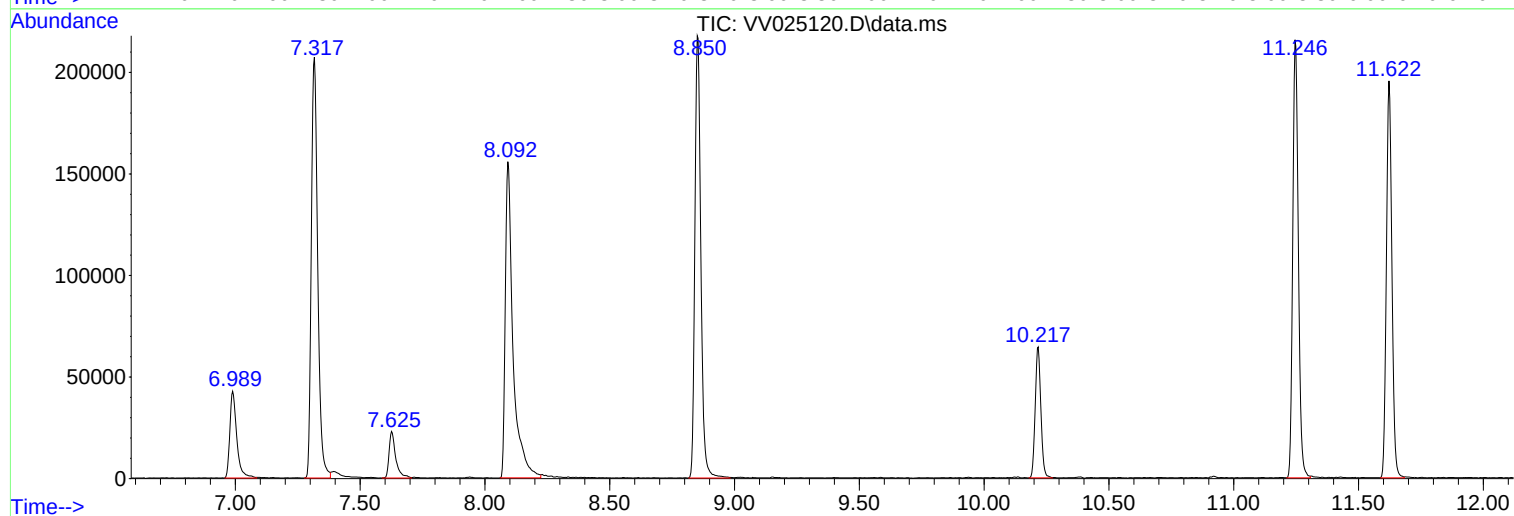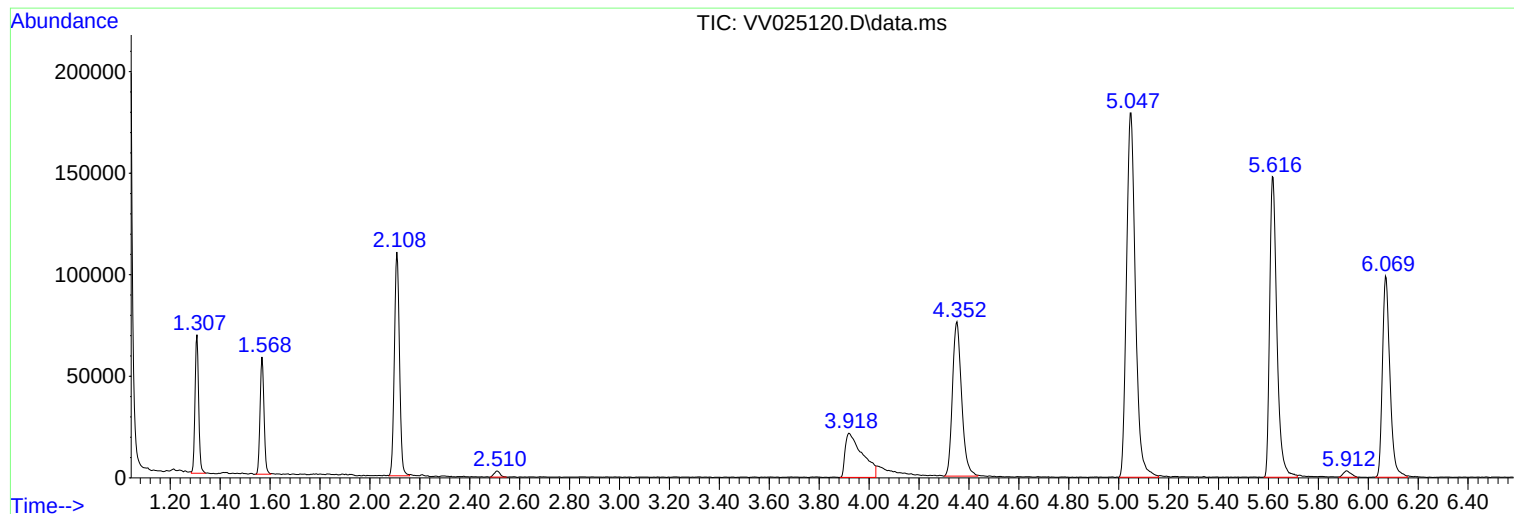

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032222\
Data File : VV025120.D
Acq On : 22 Mar 2022 11:07
Operator : SY/MD
Sample : VV0322WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK321

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032222\
Data File : VV025120.D
Acq On : 22 Mar 2022 11:07
Operator : SY/MD
Sample : VV0322WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK321

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc