


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032222\
Data File : VV025118.D
Acq On : 22 Mar 2022 09:33
Operator : SY/MD
Sample : BFB284
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB284

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Mar 23 01:08:13 2022

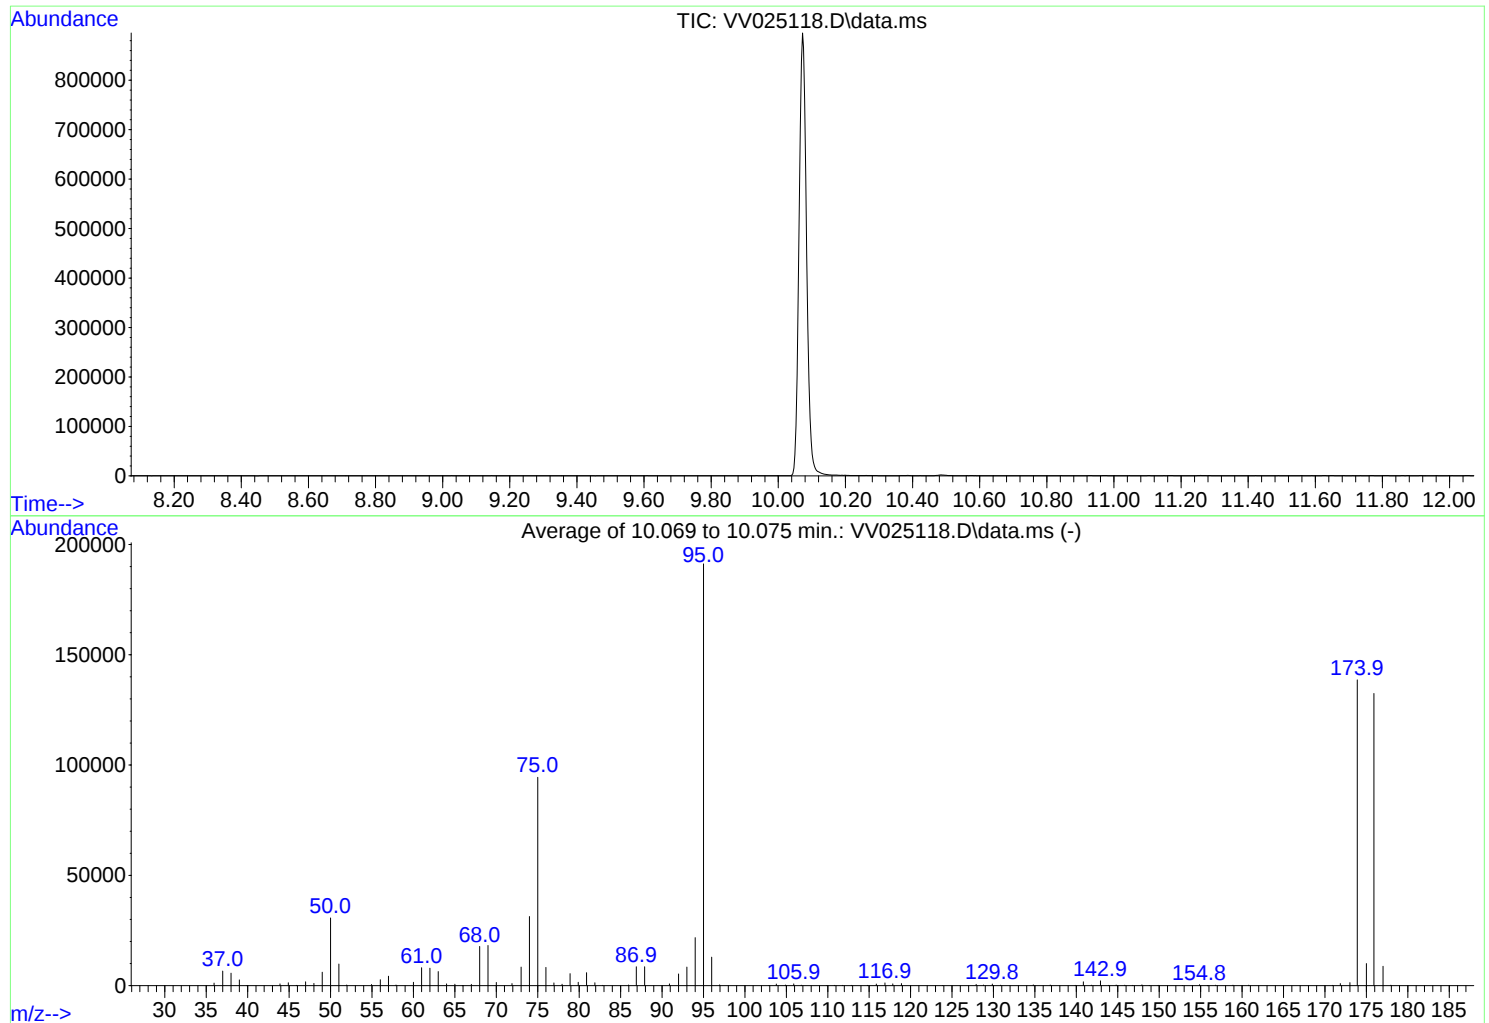

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	30707	PASS
75	95	30	80	49.4	94451	PASS
95	95	100	100	100.0	191232	PASS
96	95	5	9	6.8	12911	PASS
173	174	0.00	2	1.0	1356	PASS
174	95	50	120	72.5	138613	PASS
175	174	5	9	7.2	10006	PASS
176	174	95	105	95.5	132435	PASS
177	176	5	10	6.6	8774	PASS

m/z	Abundance
40.00	194.0
43.90	213.0

Instrument :
MSVOA_V
ClientSampleId :
BFB284

m/z	Abundance
36.00	1110.0
37.00	6584.0
38.00	5653.0
39.00	2485.0
39.90	187.0
44.00	981.0
44.90	1287.0
45.90	187.0
47.00	1631.0
48.00	964.0
49.00	6209.0
50.00	30344.0
51.00	9627.0
51.90	325.0
55.00	425.0
56.00	2600.0
57.00	4322.0
57.90	288.0
60.00	1644.0
61.00	7637.0
62.00	7941.0
63.00	6537.0
64.00	812.0
65.00	764.0
65.90	105.0
67.00	520.0
68.00	17784.0
69.00	18112.0
70.00	1392.0
71.90	873.0
73.00	8137.0
74.00	30744.0
75.00	92584.0
76.00	8271.0
76.90	1141.0
77.90	640.0
78.90	5064.0
79.90	1461.0
80.90	5810.0
81.90	1344.0
82.90	112.0
85.90	283.0
86.90	8281.0
87.90	8373.0
90.90	707.0
92.00	5296.0
93.00	8316.0
94.00	20952.0
95.00	185728.0
96.00	12792.0
97.00	391.0
103.80	713.0
104.90	288.0
105.90	832.0
106.80	196.0
110.80	166.0
112.80	131.0
114.70	183.0
115.80	759.0
116.90	1112.0
117.90	662.0
118.90	936.0
127.90	552.0
128.80	280.0
129.90	709.0
130.80	258.0
134.80	363.0
136.90	241.0
139.80	171.0
140.80	1650.0
141.80	180.0
142.90	2197.0
143.90	125.0
144.80	331.0
145.80	263.0
146.70	118.0
147.90	380.0
149.90	180.0
154.00	114.0
154.80	401.0
155.80	104.0
156.80	201.0
158.90	188.0
160.80	210.0
170.90	127.0
171.90	974.0
173.00	1368.0
173.90	131040.0
175.00	9798.0
175.90	124600.0
177.00	8453.0
177.90	255.0

Instrument :
MSVOA_V
ClientSampleId :
BFB284

m/z	Abundance
36.00	1201.0
37.00	6827.0
38.00	5816.0
39.00	2700.0
39.90	200.0
44.00	1051.0
44.90	1357.0
45.90	144.0
47.00	1807.0
48.00	1101.0
49.00	6272.0
50.00	31688.0
51.00	10167.0
51.90	333.0
55.00	524.0
56.00	2825.0
57.00	4373.0
57.90	283.0
60.00	1588.0
61.00	8401.0
62.00	8150.0
63.00	6588.0
64.00	832.0
65.00	703.0
67.00	598.0
68.00	18296.0
69.00	18904.0
70.00	1559.0
71.90	938.0
73.00	8755.0
74.00	32400.0
75.00	97704.0
76.00	8612.0
76.90	1250.0
77.90	680.0
78.90	5565.0
79.90	1534.0
80.90	6085.0
81.90	1392.0
82.90	144.0
85.90	309.0
86.90	8847.0
87.90	8814.0
90.90	795.0
92.00	5524.0
93.00	8772.0
94.00	22472.0
95.00	197504.0
96.00	13325.0
97.00	419.0
102.90	100.0
103.80	760.0
104.90	338.0
105.90	850.0
106.80	227.0
109.90	102.0
110.80	181.0
111.80	151.0
112.90	148.0
114.80	181.0
115.90	776.0
116.90	1296.0
117.80	825.0
118.90	938.0
123.80	123.0
127.90	613.0
128.80	323.0
129.90	724.0
130.90	230.0
134.80	360.0
136.80	278.0
139.80	148.0
140.90	1789.0
141.80	239.0
142.90	2234.0
143.90	132.0
144.80	317.0
145.80	234.0
146.80	118.0
147.90	418.0
148.80	145.0
149.90	191.0
152.80	114.0
154.00	116.0
154.80	423.0
156.80	209.0
158.90	221.0
160.80	254.0
170.90	168.0
171.80	964.0
173.00	1401.0
173.90	143232.0

Instrument :
MSVOA_V
ClientSampleId :
BFB284

175.00	10301.0
175.90	137024.0
177.00	9078.0
177.90	234.0

Instrument :
MSVOA_V
ClientSampleId :
BFB284

m/z	Abundance
35.90	1196.0
37.00	6304.0
38.00	5461.0
39.00	2573.0
39.90	255.0
43.90	1061.0
44.90	1277.0
45.90	114.0
47.00	1867.0
48.00	1065.0
49.00	5898.0
50.00	30088.0
51.00	9529.0
52.00	320.0
54.90	518.0
56.00	2736.0
57.00	4182.0
57.90	231.0
60.00	1440.0
61.00	8367.0
62.00	7748.0
63.00	6013.0
64.00	758.0
65.00	587.0
67.00	586.0
68.00	17232.0
69.00	17672.0
70.00	1466.0
71.90	965.0
73.00	8396.0
74.00	30776.0
75.00	93064.0
76.00	7880.0
77.00	1256.0
78.00	745.0
78.90	5609.0
79.90	1551.0
80.90	5718.0
81.90	1293.0
82.80	196.0
86.00	300.0
86.90	8655.0
87.90	8558.0
90.90	804.0
92.00	5075.0
93.00	8253.0
94.00	21992.0
95.00	190464.0
96.00	12615.0
96.90	381.0
102.90	101.0
103.80	763.0
104.90	343.0
105.90	793.0
106.80	239.0
109.90	109.0
110.80	161.0
111.80	186.0
112.90	165.0
114.90	167.0
115.90	671.0
116.90	1307.0
117.80	827.0
118.90	911.0
123.90	134.0
127.90	658.0
128.80	319.0
129.80	675.0
130.90	203.0
134.80	320.0
136.80	311.0
139.90	151.0
140.90	1769.0
141.80	245.0
142.90	2122.0
143.90	116.0
144.80	259.0
145.90	207.0
146.90	132.0
147.90	405.0
148.80	160.0
149.80	156.0
152.80	121.0
154.90	446.0
156.80	231.0
158.90	213.0
160.80	279.0
170.90	178.0
171.90	891.0
173.00	1298.0
173.90	141568.0
175.00	9918.0

Instrument :
MSVOA_V
ClientSampleId :
BFB284

175.90	135680.0
177.00	8790.0
178.00	217.0

Instrument :
MSVOA_V
ClientSampleId :
BFB284