
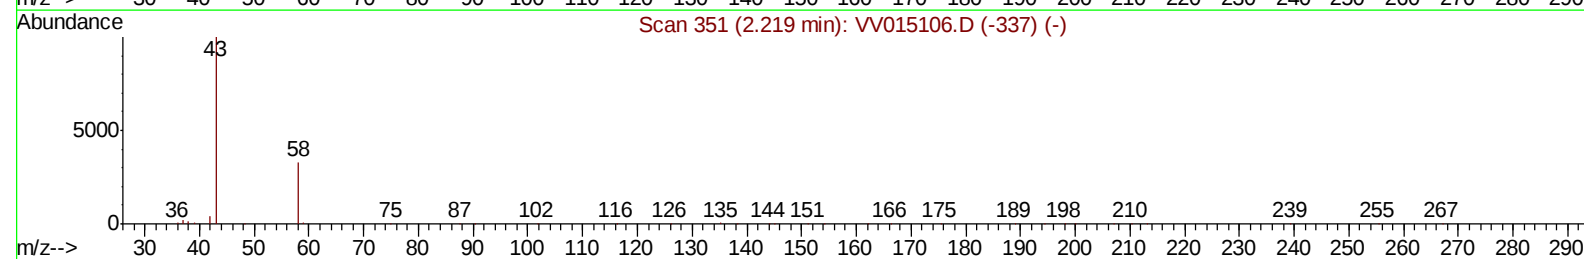
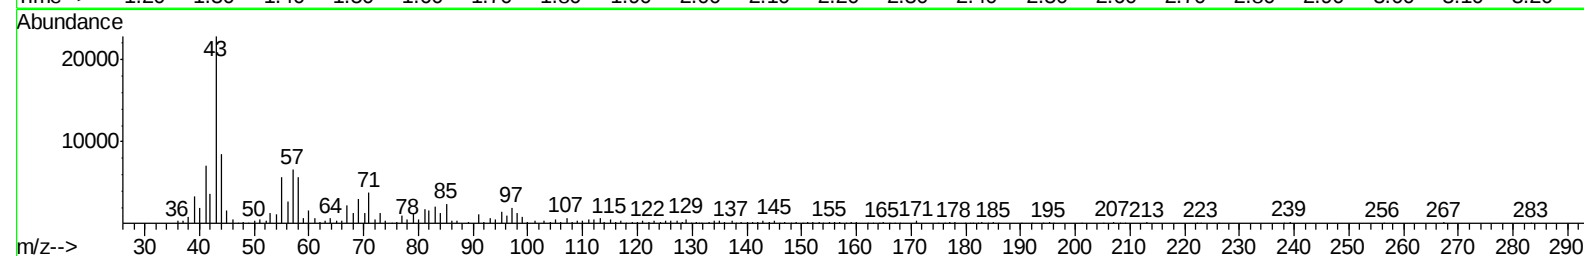


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032320\
 Data File : VV015105.D
 Acq On : 23 Mar 2020 23:34
 Operator : SY/MD
 Sample : VSTD01061
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 24 01:58:54 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 24 01:56:31 2020
 Response via : Initial Calibration

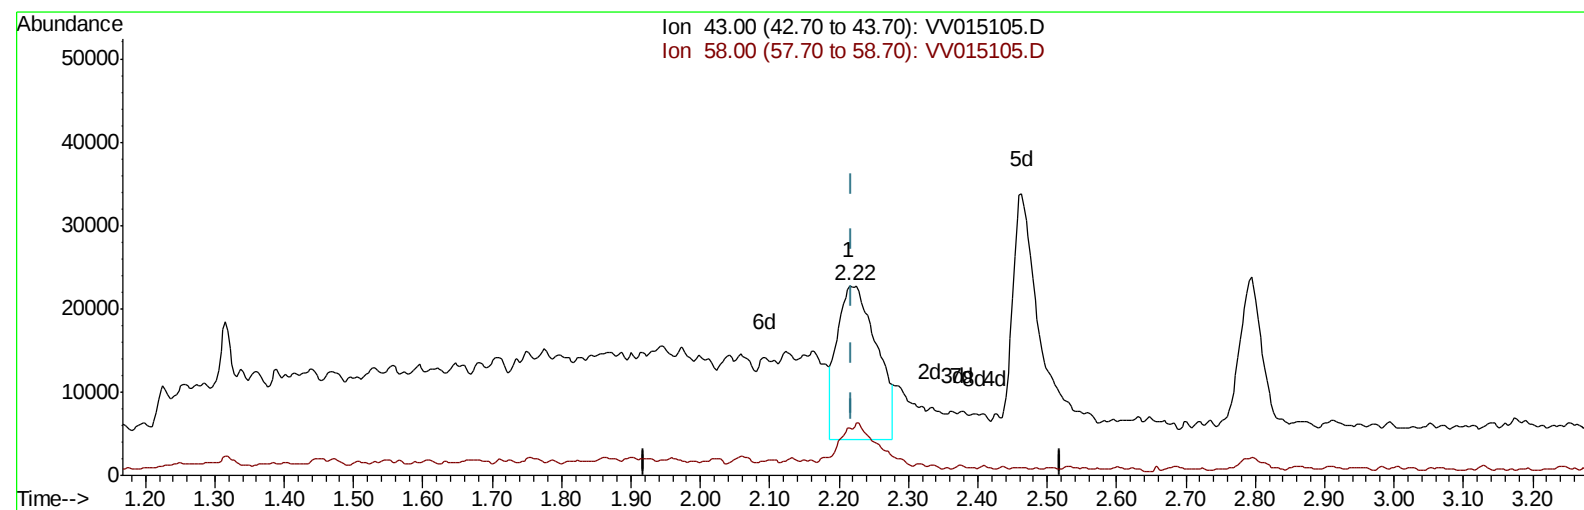

TIC: VV015105.D

(13) Acetone (T)

2.216min (-0.003) 34.00ug/L m

response 72712

Ion	Exp%	Act%
43.00	100	100
58.00	32.10	6.09
0.00	0.00	0.00
0.00	0.00	0.00