


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032320\
 Data File : VV015103.D
 Acq On : 23 Mar 2020 21:57
 Operator : SY/MD
 Sample : BFB70
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB70

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
 Title : VOC Analysis
 Last Update : Tue Mar 24 10:01:15 2020

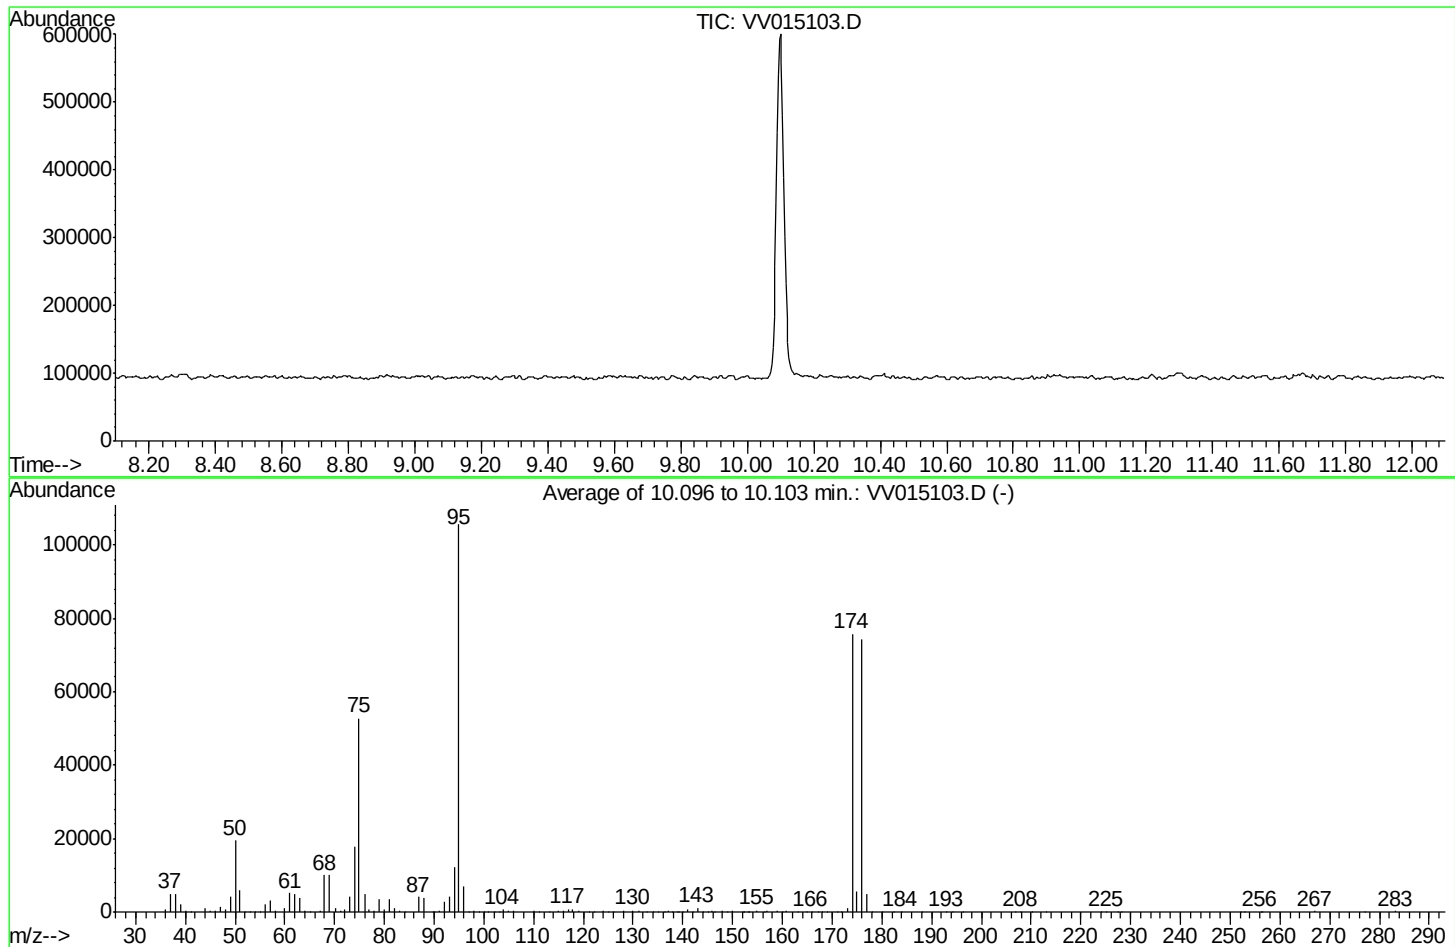

AutoFind: Scans 2801, 2802, 2803; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	19506	PASS
75	95	30	80	49.9	52716	PASS
95	95	100	100	100.0	105586	PASS
96	95	5	9	6.5	6859	PASS
173	174	0.00	2	1.5	1168	PASS
174	95	50	120	71.8	75802	PASS
175	174	5	9	7.5	5701	PASS
176	174	95	101	98.0	74298	PASS
177	176	5	9	6.7	4951	PASS

m/z	Abundance
35.90	264.0
37.00	244.0
38.00	369.0
39.00	1786.0
40.00	1581.0
41.10	4804.0
42.10	2265.0
43.00	7452.0
44.00	5090.0
45.00	1648.0
46.10	288.0
47.80	163.0
50.00	475.0
51.00	502.0
52.00	268.0
52.90	776.0
54.00	705.0
55.10	4405.0
56.10	2313.0
57.10	5980.0
58.00	1046.0
59.00	641.0
60.00	1498.0
61.00	476.0
62.00	179.0
62.90	145.0
63.90	130.0
65.00	383.0
66.00	287.0
67.10	1309.0
68.00	1031.0
69.10	3088.0
70.10	1360.0
71.10	3534.0
72.10	478.0
73.00	1319.0
74.00	383.0
74.90	110.0
76.00	117.0
77.00	413.0
78.00	311.0
79.00	633.0
80.10	311.0
81.00	1215.0
82.00	1014.0
83.00	1645.0
84.00	1088.0
85.10	2798.0
86.10	443.0
86.90	504.0
88.50	108.0
91.00	586.0
92.10	291.0
93.00	530.0
94.00	371.0
95.10	744.0
96.00	988.0
97.10	1586.0
98.00	1041.0
99.10	825.0
100.20	116.0
101.00	203.0
103.00	231.0
103.80	148.0
105.10	310.0
105.90	108.0
106.90	392.0
107.90	260.0
109.00	527.0
110.10	220.0
111.10	650.0
112.10	604.0
113.10	582.0
114.00	274.0
115.00	383.0
116.10	168.0
116.90	226.0
119.00	325.0
120.00	191.0
121.10	320.0
122.10	225.0
123.00	308.0
124.20	139.0
125.10	291.0
126.00	368.0
127.10	442.0
128.10	255.0
129.10	609.0
132.00	166.0
133.00	244.0
134.20	154.0
135.10	182.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

135.90	223.0
137.10	176.0
138.00	146.0
139.10	189.0
140.20	167.0
141.10	390.0
142.00	106.0
143.10	207.0
145.10	184.0
147.10	137.0
148.90	198.0
150.20	107.0
151.80	136.0
154.10	228.0
155.20	202.0
157.20	115.0
158.30	127.0
160.10	113.0
162.10	142.0
169.10	117.0
171.10	187.0
173.00	214.0
178.00	119.0
182.10	173.0
183.00	178.0
185.10	189.0
199.00	137.0
200.10	127.0
206.90	243.0
207.50	100.0
216.90	123.0
238.30	130.0
239.10	282.0
239.90	111.0
255.20	285.0
267.30	305.0
284.30	166.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
36.00	827.0
37.00	4944.0
38.00	4725.0
39.00	3595.0
40.00	1812.0
41.10	5128.0
42.10	1888.0
43.10	6673.0
44.00	6121.0
45.00	2146.0
46.00	518.0
47.10	1660.0
48.00	925.0
49.00	4147.0
50.00	18376.0
51.00	6036.0
52.00	427.0
53.00	904.0
54.00	810.0
55.00	4540.0
56.00	4447.0
57.10	8564.0
58.00	1221.0
59.00	456.0
60.00	2729.0
61.00	5087.0
62.00	4938.0
63.00	3783.0
63.90	507.0
65.00	523.0
66.10	247.0
67.00	1587.0
68.00	10448.0
69.00	12414.0
70.10	2344.0
71.10	4032.0
72.00	1200.0
73.00	5144.0
74.00	16688.0
75.00	49688.0
76.00	4556.0
77.00	817.0
78.00	717.0
79.00	3799.0
80.00	1081.0
81.00	4716.0
82.00	1924.0
83.10	2011.0
84.00	1130.0
85.10	2689.0
87.00	4106.0
88.00	3815.0
90.10	140.0
91.00	962.0
92.00	2954.0
93.00	4812.0
94.00	11983.0
95.00	100840.0
96.00	7138.0
97.00	1648.0
98.00	1349.0
99.10	789.0
100.00	179.0
101.00	298.0
102.10	191.0
103.00	475.0
104.00	604.0
105.00	640.0
105.80	529.0
107.10	412.0
109.10	446.0
110.00	548.0
111.10	585.0
112.00	605.0
113.10	571.0
113.90	183.0
115.10	612.0
115.90	621.0
116.90	828.0
117.90	532.0
118.90	725.0
119.90	122.0
121.00	388.0
122.00	260.0
122.90	269.0
124.00	329.0
125.00	378.0
126.00	466.0
127.00	300.0
128.00	496.0
129.00	556.0
129.90	476.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

131.10	251.0
132.00	118.0
133.10	235.0
134.10	109.0
135.00	230.0
136.20	147.0
137.20	339.0
138.10	157.0
139.00	218.0
140.20	234.0
140.90	1085.0
141.90	246.0
142.90	1312.0
144.90	184.0
145.80	160.0
146.30	119.0
147.00	146.0
147.80	396.0
149.00	332.0
149.90	209.0
152.30	190.0
152.90	118.0
153.90	114.0
154.90	403.0
156.30	108.0
156.90	271.0
159.00	162.0
160.10	119.0
160.90	223.0
164.80	130.0
165.80	195.0
168.00	151.0
168.90	216.0
171.30	247.0
173.10	1527.0
174.00	73784.0
175.00	5235.0
176.00	71912.0
177.00	4985.0
178.00	240.0
182.80	147.0
185.20	158.0
196.20	114.0
207.00	213.0
207.90	142.0
210.10	112.0
213.10	172.0
225.10	226.0
227.30	120.0
228.20	102.0
239.20	264.0
255.40	114.0
256.20	110.0
256.40	111.0
267.00	179.0
283.30	222.0
284.30	131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
36.00	961.0
37.00	5431.0
38.00	5242.0
39.00	3771.0
40.00	2002.0
41.10	4948.0
42.10	1778.0
43.10	6623.0
44.00	6193.0
45.00	2205.0
46.00	465.0
47.10	1608.0
48.00	1013.0
49.00	4428.0
50.00	20480.0
51.00	6459.0
52.00	452.0
53.00	852.0
54.00	862.0
55.10	4583.0
56.00	4364.0
57.10	9042.0
58.00	1270.0
59.00	460.0
60.00	2781.0
61.00	5813.0
62.00	5185.0
63.00	4255.0
63.90	473.0
65.00	609.0
66.10	194.0
67.10	1688.0
68.00	11278.0
69.00	13469.0
70.10	2320.0
71.10	3793.0
72.00	1196.0
73.00	5454.0
74.00	18888.0
75.00	54632.0
76.00	4959.0
77.00	1031.0
78.00	812.0
78.90	4146.0
80.00	1188.0
80.90	4954.0
82.00	2088.0
83.10	2016.0
84.00	1123.0
85.10	2736.0
85.90	289.0
87.00	4651.0
88.00	3981.0
89.90	122.0
90.10	119.0
91.00	1091.0
92.00	3194.0
93.00	4933.0
94.00	13397.0
95.00	109656.0
96.00	8165.0
97.00	1721.0
98.10	1467.0
99.10	868.0
100.00	213.0
100.90	232.0
102.10	145.0
103.00	405.0
103.90	790.0
105.00	615.0
105.90	647.0
107.10	373.0
108.10	122.0
109.10	372.0
110.00	565.0
111.00	720.0
112.00	569.0
113.10	615.0
113.90	181.0
115.10	687.0
115.90	676.0
116.90	1021.0
117.90	578.0
118.90	749.0
119.90	121.0
121.10	346.0
122.10	277.0
122.90	248.0
124.00	359.0
125.00	437.0
126.00	451.0
127.00	319.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

128.00	504.0
129.00	578.0
129.90	510.0
131.10	273.0
132.00	144.0
133.10	203.0
133.90	120.0
134.90	243.0
136.30	186.0
137.20	390.0
137.90	160.0
139.00	215.0
139.90	228.0
141.00	1095.0
142.00	302.0
143.00	1344.0
143.90	107.0
144.90	209.0
145.80	207.0
147.10	107.0
147.80	416.0
149.00	409.0
149.90	190.0
152.30	229.0
153.00	129.0
153.30	124.0
153.90	163.0
154.90	361.0
156.30	115.0
157.00	285.0
159.00	236.0
160.10	181.0
160.80	284.0
163.00	118.0
164.90	112.0
165.80	156.0
167.30	103.0
168.00	153.0
168.90	196.0
171.20	237.0
173.10	1417.0
174.00	78176.0
175.00	5834.0
176.00	76840.0
177.00	5071.0
178.00	301.0
182.80	149.0
185.30	149.0
188.00	107.0
193.00	114.0
206.90	320.0
207.90	160.0
213.10	108.0
225.10	169.0
227.30	135.0
228.20	111.0
239.20	229.0
252.90	112.0
256.10	130.0
267.00	212.0
283.30	273.0
284.30	156.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
36.00	958.0
37.00	5400.0
38.00	5483.0
39.00	3889.0
40.00	2058.0
41.00	4547.0
42.10	1790.0
43.10	6801.0
44.00	6181.0
45.00	2097.0
46.00	491.0
47.00	1408.0
48.00	1008.0
49.00	4405.0
50.00	21088.0
51.00	6343.0
52.00	465.0
53.00	772.0
54.00	852.0
55.10	4593.0
56.00	4321.0
57.00	9393.0
58.00	1225.0
58.90	515.0
60.00	2617.0
61.00	5867.0
62.00	4907.0
63.00	4403.0
64.00	482.0
64.90	543.0
66.00	221.0
67.10	1717.0
68.00	11411.0
69.00	13836.0
70.10	2282.0
71.10	3744.0
72.00	1155.0
73.00	5559.0
74.00	19176.0
75.00	54160.0
76.00	5108.0
77.00	1151.0
78.10	797.0
78.90	4276.0
80.00	1261.0
80.90	4695.0
82.00	2134.0
83.10	1962.0
84.00	1129.0
85.10	2668.0
86.00	372.0
86.90	4951.0
88.00	3932.0
89.80	137.0
91.00	1248.0
92.00	3336.0
93.00	4747.0
94.00	12844.0
95.00	108496.0
96.00	8238.0
97.00	1949.0
98.10	1406.0
99.00	848.0
100.00	217.0
100.80	187.0
102.00	168.0
103.00	342.0
103.90	780.0
105.00	577.0
105.90	720.0
107.00	366.0
108.10	214.0
109.10	373.0
110.00	481.0
111.00	757.0
112.00	492.0
113.10	690.0
114.00	199.0
115.10	590.0
115.90	576.0
116.90	1174.0
117.90	575.0
119.00	665.0
119.90	120.0
121.10	274.0
122.00	285.0
122.90	218.0
124.00	316.0
125.00	446.0
126.00	365.0
127.00	368.0
127.90	433.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

129.00	620.0
129.90	486.0
131.00	312.0
132.00	103.0
132.70	204.0
133.90	213.0
134.90	342.0
136.20	187.0
137.10	398.0
137.80	168.0
138.80	189.0
139.10	188.0
139.90	276.0
141.00	1103.0
142.00	308.0
143.00	1178.0
143.90	140.0
144.90	209.0
145.90	221.0
147.20	116.0
147.80	367.0
149.00	362.0
149.90	166.0
152.10	267.0
153.00	165.0
153.90	171.0
155.00	341.0
157.00	235.0
159.00	290.0
160.10	161.0
160.80	265.0
163.00	142.0
165.00	109.0
166.00	112.0
168.00	149.0
169.00	168.0
171.30	261.0
171.90	142.0
173.00	1204.0
174.00	75448.0
175.00	6036.0
176.00	74144.0
177.00	4797.0
178.00	280.0
180.10	103.0
182.40	118.0
183.90	142.0
185.20	150.0
194.20	115.0
199.10	124.0
206.90	345.0
207.90	119.0
224.10	112.0
239.10	206.0
252.00	103.0
252.90	147.0
256.20	127.0
267.10	203.0
277.10	117.0
283.20	195.0
284.30	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70