
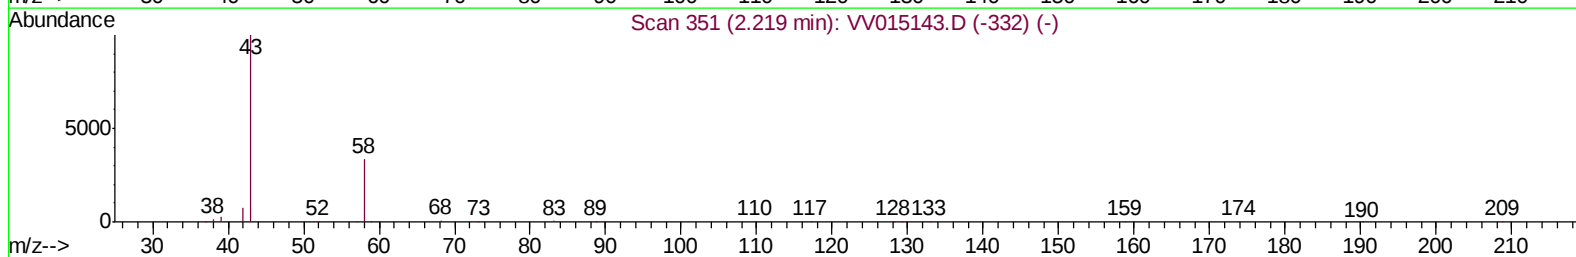
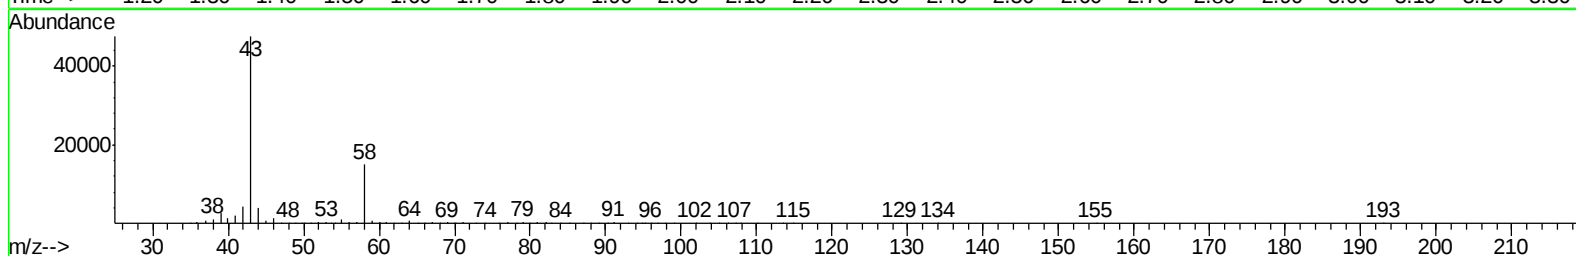


Data File : VV015163.D
Acq On : 26 Mar 2020 02:59
Operator : SY/MD
Sample : VSTDCCC050EC
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 04:26:57 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 26 02:00:02 2020
Response via : Initial Calibration

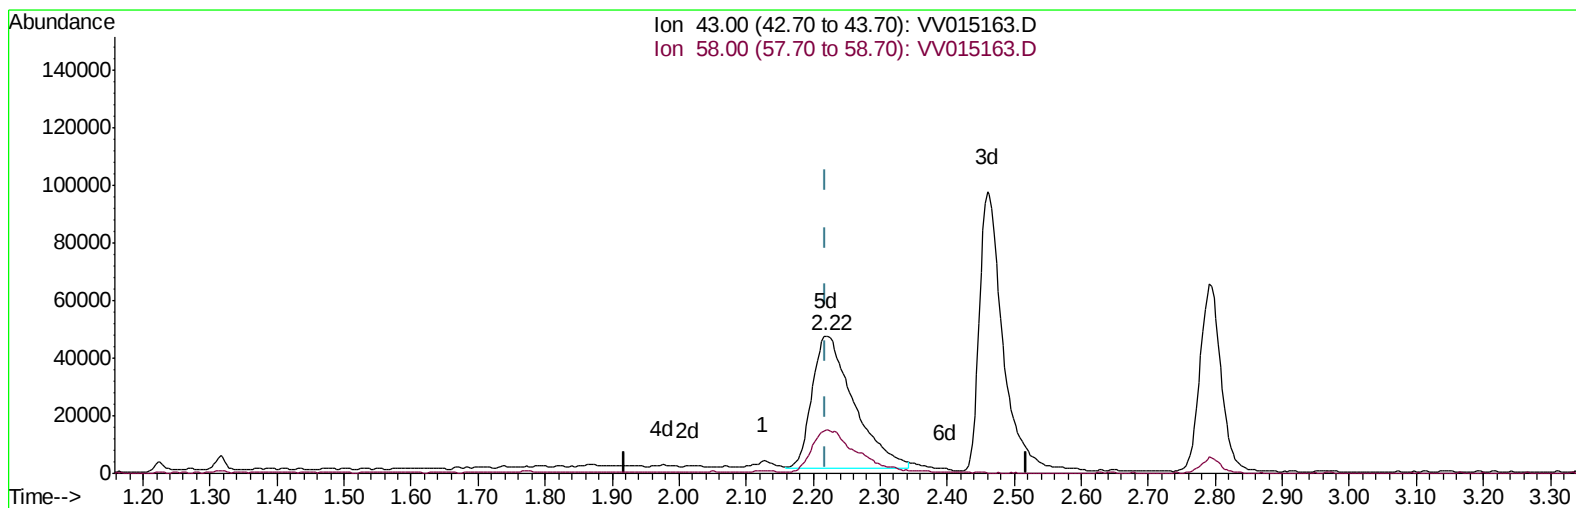

TIC: VV015163.D

(13) Acetone (T)

2.219min (+0.000) 103.78ug/L m

response 198672

Ion	Exp%	Act%
43.00	100	100
58.00	14.20	0.06
0.00	0.00	0.00
0.00	0.00	0.00