

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032520\
 Data File : VV015145.D
 Acq On : 25 Mar 2020 19:42
 Operator : SY/MD
 Sample : L1968-10 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CODE0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	81	rVB	344084	346763	9.70%	1.655%
2	1.579	146	152	162	rVB	286847	334346	9.35%	1.596%
3	2.119	314	320	332	rVB	609811	834625	23.34%	3.983%
4	3.116	628	630	631	rBV2	1953	923	0.03%	0.004%
5	3.486	743	745	747	rBV3	1524	796	0.02%	0.004%
6	3.573	769	772	773	rBV3	1929	1111	0.03%	0.005%
7	3.666	797	801	803	rBV5	2206	1841	0.05%	0.009%
8	3.704	808	813	815	rBV6	1865	1432	0.04%	0.007%
9	3.762	828	831	833	rVB4	2235	1113	0.03%	0.005%
10	3.778	833	836	837	rBV3	2610	1673	0.05%	0.008%
11	3.801	841	843	846	rVB3	2984	1663	0.05%	0.008%
12	3.856	857	860	861	rBV3	1388	843	0.02%	0.004%
13	3.881	865	868	873	rBV7	1793	1610	0.05%	0.008%
14	3.939	873	886	939	rBV2	130586	619077	17.31%	2.954%
15	4.376	1009	1022	1046	rVB	356244	868794	24.30%	4.146%
16	4.553	1074	1077	1078	rBV3	2645	1656	0.05%	0.008%
17	4.585	1085	1087	1089	rBV2	1858	1068	0.03%	0.005%
18	4.862	1168	1173	1177	rBV7	1960	2627	0.07%	0.013%
19	4.917	1186	1190	1192	rBV5	1723	1159	0.03%	0.006%
20	4.949	1198	1200	1203	rBV4	1516	1050	0.03%	0.005%
21	5.013	1217	1220	1221	rBV3	2448	1297	0.04%	0.006%
22	5.074	1222	1239	1252	rBV2	864896	2199194	61.50%	10.495%
23	5.643	1403	1416	1433	rBV	673093	1331839	37.24%	6.356%
24	6.097	1543	1557	1584	rBV	493303	1014361	28.37%	4.841%
25	6.399	1648	1651	1653	rVB3	1875	1016	0.03%	0.005%
26	6.528	1689	1691	1694	rBV4	1822	1026	0.03%	0.005%
27	6.556	1698	1700	1703	rBV3	1529	873	0.02%	0.004%
28	6.640	1723	1726	1727	rBV2	3185	1718	0.05%	0.008%
29	6.733	1752	1755	1757	rBV4	1925	1298	0.04%	0.006%
30	6.884	1799	1802	1804	rBV3	1797	1317	0.04%	0.006%
31	7.010	1828	1841	1868	rBV	289691	527526	14.75%	2.518%
32	7.338	1929	1943	1962	rBV	1039026	1802143	50.40%	8.601%
33	7.515	1996	1998	2003	rVB5	2446	1622	0.05%	0.008%
34	7.643	2027	2038	2055	rBV	209952	361766	10.12%	1.726%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032520\
 Data File : VV015145.D
 Acq On : 25 Mar 2020 19:42
 Operator : SY/MD
 Sample : L1968-10 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CODE0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
 Title : VOC Analysis

35	7.814	2089	2091	2095	rBV4	1877	1330	0.04%	0.006%
36	7.849	2099	2102	2104	rBV3	2023	1436	0.04%	0.007%
37	7.945	2128	2132	2139	rBV9	1916	3005	0.08%	0.014%
38	7.974	2139	2141	2143	rBV3	1592	861	0.02%	0.004%
39	8.116	2174	2185	2217	rBV	655381	1331290	37.23%	6.353%
40	8.344	2254	2256	2258	rBV3	1712	968	0.03%	0.005%
41	8.515	2304	2309	2311	rBV5	1906	1631	0.05%	0.008%
42	8.556	2320	2322	2326	rBV4	2200	922	0.03%	0.004%
43	8.643	2345	2349	2351	rBV6	1665	1277	0.04%	0.006%
44	8.724	2369	2374	2377	rBV6	2110	1428	0.04%	0.007%
45	8.765	2385	2387	2390	rBV4	1722	1077	0.03%	0.005%
46	8.875	2409	2421	2423	rBV	1152024	1477656	41.32%	7.052%
47	9.080	2482	2485	2488	rVB5	1901	1068	0.03%	0.005%
48	9.341	2564	2566	2568	rBV3	2048	1063	0.03%	0.005%
49	9.656	2660	2664	2667	rVB6	2050	1288	0.04%	0.006%
50	9.685	2670	2673	2675	rBV4	2150	1210	0.03%	0.006%
51	9.772	2698	2700	2704	rBV5	2071	1768	0.05%	0.008%
52	9.990	2766	2768	2771	rBV4	1576	987	0.03%	0.005%
53	10.183	2823	2828	2831	rVB7	2318	1768	0.05%	0.008%
54	10.238	2831	2845	2861	rBV	732084	1152747	32.24%	5.501%
55	10.360	2882	2883	2889	rVB4	2798	1742	0.05%	0.008%
56	10.392	2889	2893	2896	rBV4	2939	2934	0.08%	0.014%
57	10.431	2902	2905	2909	rBV6	2144	2107	0.06%	0.010%
58	10.527	2928	2935	2939	rBV9	2312	3419	0.10%	0.016%
59	10.643	2969	2971	2976	rVB6	3069	2115	0.06%	0.010%
60	10.685	2982	2984	2988	rVB5	2796	1570	0.04%	0.007%
61	10.711	2988	2992	2996	rBV7	2380	2277	0.06%	0.011%
62	10.762	3006	3008	3013	rVB6	1787	1251	0.03%	0.006%
63	10.875	3041	3043	3049	rVB7	3096	2472	0.07%	0.012%
64	10.936	3059	3062	3065	rBV4	2353	1963	0.05%	0.009%
65	10.977	3071	3075	3079	rBV6	1881	2036	0.06%	0.010%
66	11.003	3079	3083	3086	rVB5	1988	1277	0.04%	0.006%
67	11.058	3098	3100	3103	rBV4	1827	1168	0.03%	0.006%
68	11.090	3106	3110	3115	rBV6	2212	1694	0.05%	0.008%
69	11.203	3129	3145	3155	rBV	160799	252549	7.06%	1.205%
70	11.273	3156	3167	3171	rBV	1102120	1820628	50.91%	8.689%
71	11.566	3252	3258	3262	rBV9	1662	1803	0.05%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032520\
 Data File : VV015145.D
 Acq On : 25 Mar 2020 19:42
 Operator : SY/MD
 Sample : L1968-10 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CODE0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
 Title : VOC Analysis

72	11.588	3262	3265	3270	rBV7	2479	2183	0.06%	0.010%
73	11.662	3271	3288	3306	rBV2	1533605	3575910	100.00%	17.066%
74	11.846	3342	3345	3350	rBV7	2332	1655	0.05%	0.008%
75	11.945	3372	3376	3383	rVB9	2257	2160	0.06%	0.010%
76	11.984	3384	3388	3390	rVV4	2038	1473	0.04%	0.007%
77	12.010	3393	3396	3400	rBV6	2071	1434	0.04%	0.007%
78	12.026	3400	3401	3404	rBV3	1385	794	0.02%	0.004%
79	12.106	3422	3426	3429	rBV6	2392	1674	0.05%	0.008%
80	12.122	3429	3431	3434	rBV4	1990	1263	0.04%	0.006%
81	12.199	3448	3455	3456	rBV7	1745	1899	0.05%	0.009%
82	12.309	3482	3489	3491	rBV7	2438	3180	0.09%	0.015%
83	12.373	3505	3509	3511	rBV5	2906	2314	0.06%	0.011%
84	12.492	3544	3546	3548	rBV3	3030	1867	0.05%	0.009%
85	12.576	3569	3572	3575	rBV4	2629	2106	0.06%	0.010%
86	12.624	3585	3587	3591	rBV5	2326	1317	0.04%	0.006%
87	12.672	3594	3602	3610	rVB5	8548	12598	0.35%	0.060%
88	12.733	3617	3621	3624	rBV5	2350	1996	0.06%	0.010%
89	12.756	3624	3628	3629	rBV3	3157	2103	0.06%	0.010%
90	12.849	3655	3657	3659	rBV3	1981	1239	0.03%	0.006%
91	12.897	3669	3672	3675	rVB5	2580	1421	0.04%	0.007%
92	12.920	3675	3679	3682	rBV6	3272	3214	0.09%	0.015%
93	13.022	3708	3711	3717	rBV7	2625	2847	0.08%	0.014%
94	13.071	3723	3726	3728	rBV3	1858	1201	0.03%	0.006%
95	13.283	3781	3792	3810	rBV	497710	760941	21.28%	3.631%
96	13.768	3934	3943	3953	rVB	129537	200207	5.60%	0.955%
97	13.916	3985	3989	3992	rBV6	1929	1222	0.03%	0.006%
98	14.267	4096	4098	4099	rBV2	1822	830	0.02%	0.004%
99	14.492	4164	4168	4171	rBV5	2846	2449	0.07%	0.012%
100	14.582	4193	4196	4199	rBV5	2397	1456	0.04%	0.007%


Sum of corrected areas: 20953904

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032520\
Data File : VV015145.D
Acq On : 25 Mar 2020 19:42
Operator : SY/MD
Sample : L1968-10 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CODE0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

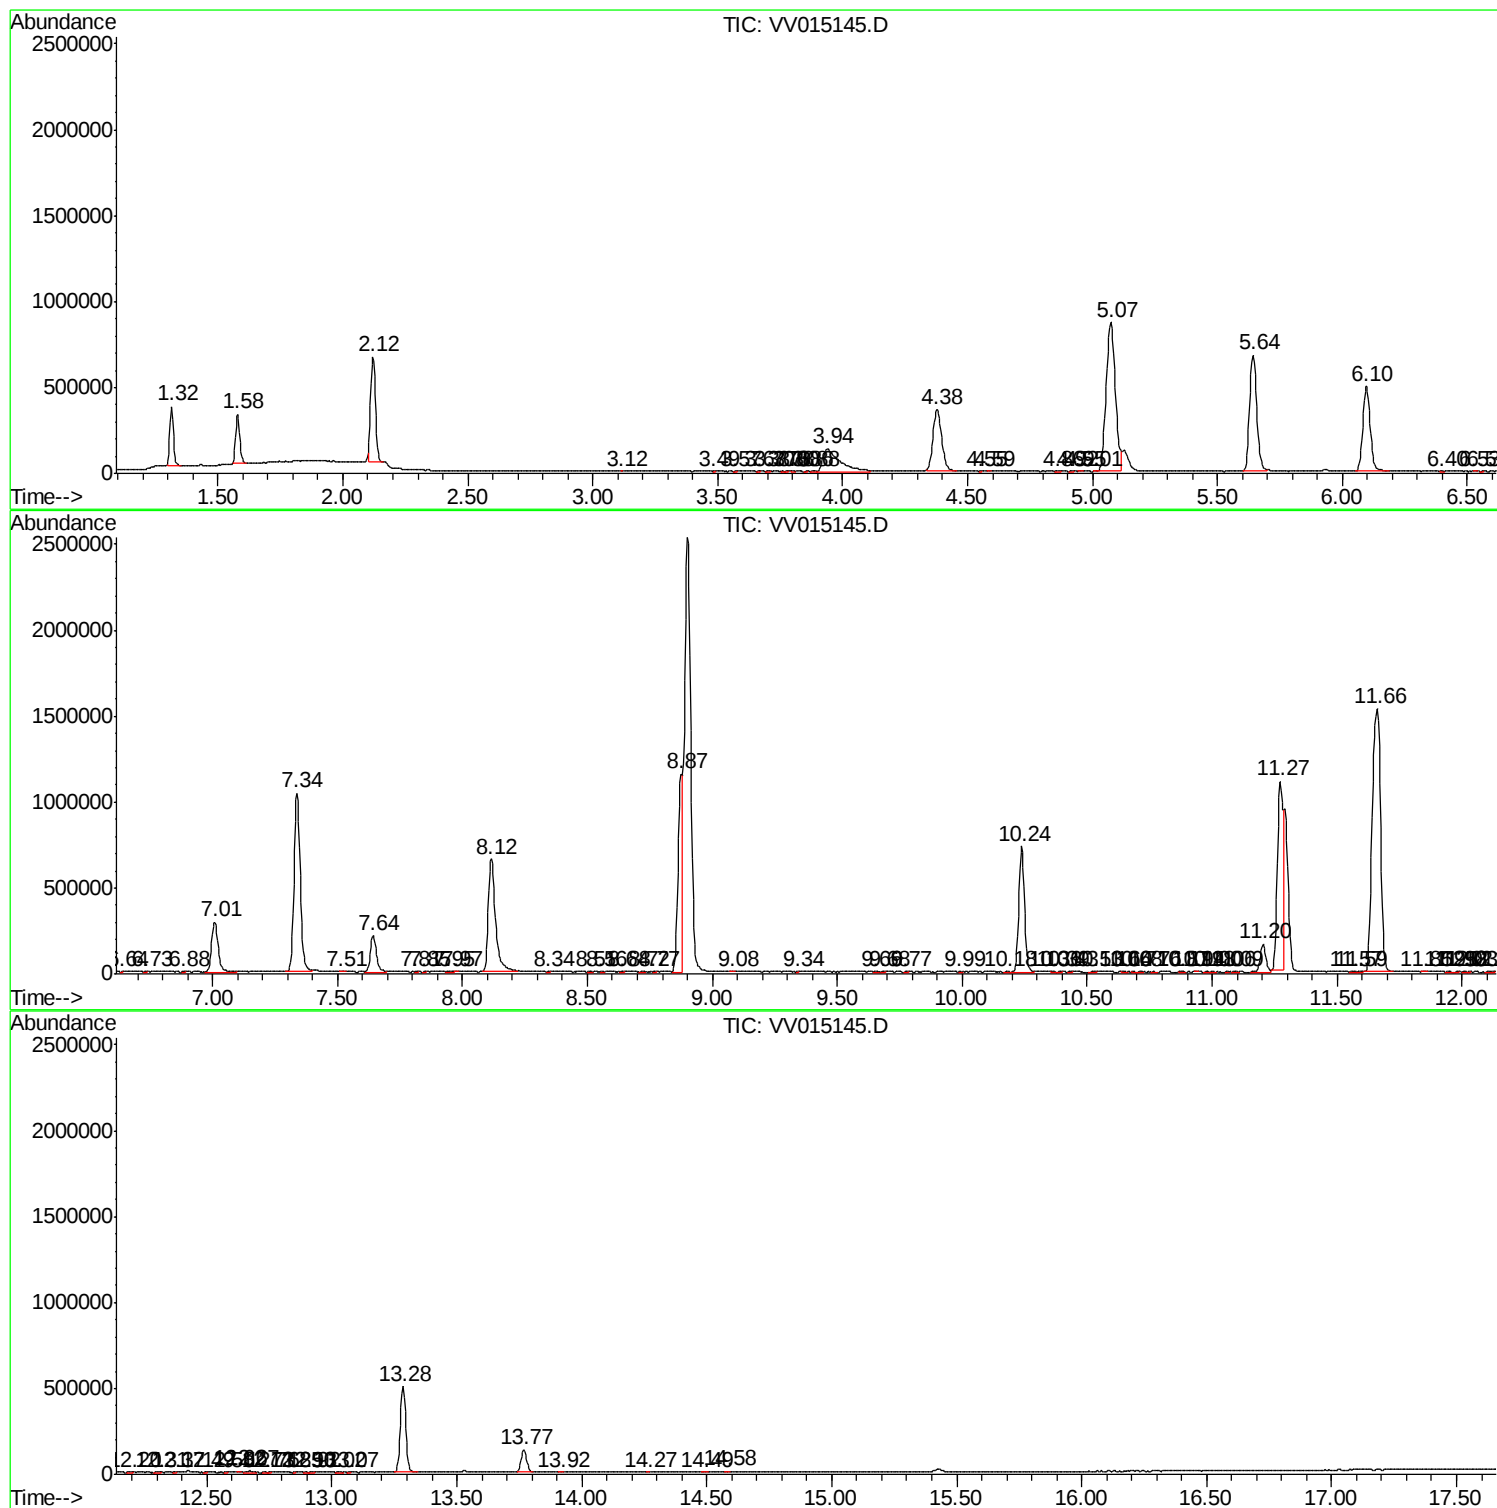

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032520\
Data File : VV015145.D
Acq On : 25 Mar 2020 19:42
Operator : SY/MD
Sample : L1968-10 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CODE0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032520\
Data File : VV015145.D
Acq On : 25 Mar 2020 19:42
Operator : SY/MD
Sample : L1968-10 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DE0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc