

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032520\
 Data File : VV015147.D
 Acq On : 25 Mar 2020 20:31
 Operator : SY/MD
 Sample : VIBLK70
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK70

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB	355598	355187	16.32%	1.961%
2	1.579	146	152	165	rVB	298186	346702	15.93%	1.914%
3	2.119	314	320	346	rVB	651699	1032672	47.46%	5.702%
4	3.393	714	716	718	rBV3	1429	731	0.03%	0.004%
5	3.592	775	778	782	rBV6	2684	2139	0.10%	0.012%
6	3.643	792	794	797	rBV3	1243	715	0.03%	0.004%
7	3.823	844	850	853	rBV8	2275	2650	0.12%	0.015%
8	3.865	862	863	865	rBV2	1463	634	0.03%	0.004%
9	3.939	873	886	917	rBV	125221	539562	24.80%	2.979%
10	4.380	1009	1023	1043	rVB	356004	861225	39.58%	4.756%
11	4.576	1080	1084	1088	rBV6	2894	2441	0.11%	0.013%
12	4.605	1091	1093	1094	rBV2	2023	883	0.04%	0.005%
13	5.074	1222	1239	1263	rBV2	871752	2176053	100.00%	12.016%
14	5.312	1310	1313	1316	rBV5	2122	1950	0.09%	0.011%
15	5.479	1363	1365	1367	rBV3	2109	1252	0.06%	0.007%
16	5.556	1385	1389	1392	rBV6	2325	2000	0.09%	0.011%
17	5.643	1398	1416	1438	rBV	718859	1455627	66.89%	8.038%
18	6.039	1535	1539	1540	rBV4	1529	996	0.05%	0.005%
19	6.097	1543	1557	1588	rVB	507908	1035088	47.57%	5.716%
20	6.235	1595	1600	1604	rBV6	3299	3740	0.17%	0.021%
21	6.479	1674	1676	1678	rBV3	1193	745	0.03%	0.004%
22	6.492	1678	1680	1683	rVB4	1841	953	0.04%	0.005%
23	6.643	1721	1727	1728	rBV6	2357	2273	0.10%	0.013%
24	6.724	1750	1752	1755	rVB3	1895	813	0.04%	0.004%
25	6.743	1755	1758	1760	rVB3	2526	1312	0.06%	0.007%
26	6.769	1760	1766	1771	rBV9	2221	3245	0.15%	0.018%
27	6.810	1776	1779	1781	rBV4	1596	1063	0.05%	0.006%
28	6.920	1810	1813	1817	rVB6	1651	1015	0.05%	0.006%
29	6.939	1817	1819	1820	rBV2	1857	796	0.04%	0.004%
30	7.007	1830	1840	1861	rBV	283172	507644	23.33%	2.803%
31	7.338	1931	1943	1963	rBV	1056155	1809578	83.16%	9.992%
32	7.550	2006	2009	2013	rBV4	2858	2410	0.11%	0.013%
33	7.576	2013	2017	2021	rBV6	2296	1952	0.09%	0.011%
34	7.598	2021	2024	2026	rBV4	1726	1184	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032520\
 Data File : VV015147.D
 Acq On : 25 Mar 2020 20:31
 Operator : SY/MD
 Sample : VIBLK70
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK70

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
 Title : VOC Analysis

35	7.643	2028	2038	2055	rVV	207956	348326	16.01%	1.923%
36	7.907	2117	2120	2121	rBV3	2396	1182	0.05%	0.007%
37	8.052	2163	2165	2168	rVB4	2001	1016	0.05%	0.006%
38	8.074	2170	2172	2174	rBV4	2049	1399	0.06%	0.008%
39	8.116	2174	2185	2217	rVV	657733	1313972	60.38%	7.256%
40	8.363	2257	2262	2264	rBV5	2125	1794	0.08%	0.010%
41	8.704	2363	2368	2372	rBV7	2749	3155	0.14%	0.017%
42	8.749	2379	2382	2385	rBV4	2184	1666	0.08%	0.009%
43	8.765	2385	2387	2390	rVB3	1716	778	0.04%	0.004%
44	8.785	2390	2393	2398	rVB7	2472	1503	0.07%	0.008%
45	8.817	2398	2403	2406	rBV7	2276	2351	0.11%	0.013%
46	8.875	2409	2421	2445	rVV	1091470	1806270	83.01%	9.974%
47	9.138	2500	2503	2504	rBV3	2011	1067	0.05%	0.006%
48	9.203	2520	2523	2526	rBV5	2610	2020	0.09%	0.011%
49	9.289	2547	2550	2555	rVB7	2042	2155	0.10%	0.012%
50	9.315	2555	2558	2559	rBV3	1454	632	0.03%	0.003%
51	9.338	2563	2565	2569	rVB5	2040	1146	0.05%	0.006%
52	9.511	2616	2619	2621	rBV3	1374	788	0.04%	0.004%
53	9.553	2625	2632	2634	rBV8	3129	3302	0.15%	0.018%
54	9.669	2665	2668	2672	rVB5	2923	2318	0.11%	0.013%
55	9.701	2672	2678	2683	rVB9	2195	2309	0.11%	0.013%
56	9.743	2688	2691	2695	rVB5	1768	1070	0.05%	0.006%
57	9.765	2696	2698	2701	rBV4	1735	1027	0.05%	0.006%
58	9.804	2705	2710	2715	rVB8	2461	2510	0.12%	0.014%
59	9.865	2726	2729	2731	rBV4	1962	1413	0.06%	0.008%
60	9.910	2740	2743	2745	rBV3	1339	754	0.03%	0.004%
61	9.926	2745	2748	2749	rBV3	2047	888	0.04%	0.005%
62	9.981	2762	2765	2768	rBV3	1670	1015	0.05%	0.006%
63	10.003	2768	2772	2777	rBV8	2036	1995	0.09%	0.011%
64	10.103	2800	2803	2806	rBV5	1929	1452	0.07%	0.008%
65	10.238	2832	2845	2865	rVV	728401	1149261	52.81%	6.346%
66	10.347	2876	2879	2882	rBV5	1952	1133	0.05%	0.006%
67	10.441	2904	2908	2909	rBV4	2466	1845	0.08%	0.010%
68	10.601	2955	2958	2961	rVB3	2777	1789	0.08%	0.010%
69	10.630	2964	2967	2968	rBV3	1535	703	0.03%	0.004%
70	10.653	2971	2974	2978	rBV5	1626	1396	0.06%	0.008%
71	10.759	3005	3007	3009	rBV3	1957	989	0.05%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032520\
 Data File : VV015147.D
 Acq On : 25 Mar 2020 20:31
 Operator : SY/MD
 Sample : VIBLK70
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK70

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
 Title : VOC Analysis

72	10.810	3019	3023	3027	rVB8	1920	1968	0.09%	0.011%
73	10.839	3027	3032	3035	rBV6	2097	2568	0.12%	0.014%
74	10.916	3053	3056	3060	rVB6	1171	896	0.04%	0.005%
75	10.968	3070	3072	3077	rVB6	2422	1303	0.06%	0.007%
76	11.019	3085	3088	3093	rBV5	2665	2313	0.11%	0.013%
77	11.116	3113	3118	3119	rBV5	2585	1779	0.08%	0.010%
78	11.177	3135	3137	3139	rBV3	1759	761	0.03%	0.004%
79	11.270	3155	3166	3186	rBV	1081109	1648239	75.74%	9.101%
80	11.505	3236	3239	3242	rBV4	2655	1968	0.09%	0.011%
81	11.569	3255	3259	3261	rBV5	1730	1230	0.06%	0.007%
82	11.646	3272	3283	3300	rBV	1028759	1593359	73.22%	8.798%
83	11.997	3390	3392	3397	rVB6	1758	1076	0.05%	0.006%
84	12.016	3397	3398	3401	rVB3	1743	824	0.04%	0.005%
85	12.129	3431	3433	3438	rVB6	1776	1338	0.06%	0.007%
86	12.653	3590	3596	3597	rBV5	3380	2803	0.13%	0.015%
87	12.720	3614	3617	3621	rBV5	1487	1365	0.06%	0.008%
88	12.846	3651	3656	3658	rBV6	2759	2907	0.13%	0.016%
89	12.932	3676	3683	3689	rBV6	2851	3358	0.15%	0.019%
90	12.974	3694	3696	3698	rBV3	1127	692	0.03%	0.004%
91	12.987	3698	3700	3702	rBV3	2289	1265	0.06%	0.007%
92	13.035	3713	3715	3721	rBV7	2421	2320	0.11%	0.013%
93	13.077	3725	3728	3731	rVB4	2412	1422	0.07%	0.008%
94	13.109	3736	3738	3743	rVV6	1456	889	0.04%	0.005%
95	13.141	3745	3748	3750	rBV3	1625	1151	0.05%	0.006%
96	13.212	3766	3770	3772	rBV4	1601	1231	0.06%	0.007%
97	13.617	3894	3896	3897	rBV2	1615	683	0.03%	0.004%
98	14.341	4118	4121	4123	rBV4	2254	1622	0.07%	0.009%
99	14.382	4131	4134	4136	rVB4	3114	1589	0.07%	0.009%
100	14.395	4136	4138	4143	rBV5	1911	1208	0.06%	0.007%


Sum of corrected areas: 18109746

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032520\
Data File : VV015147.D
Acq On : 25 Mar 2020 20:31
Operator : SY/MD
Sample : VIBLK70
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK70

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

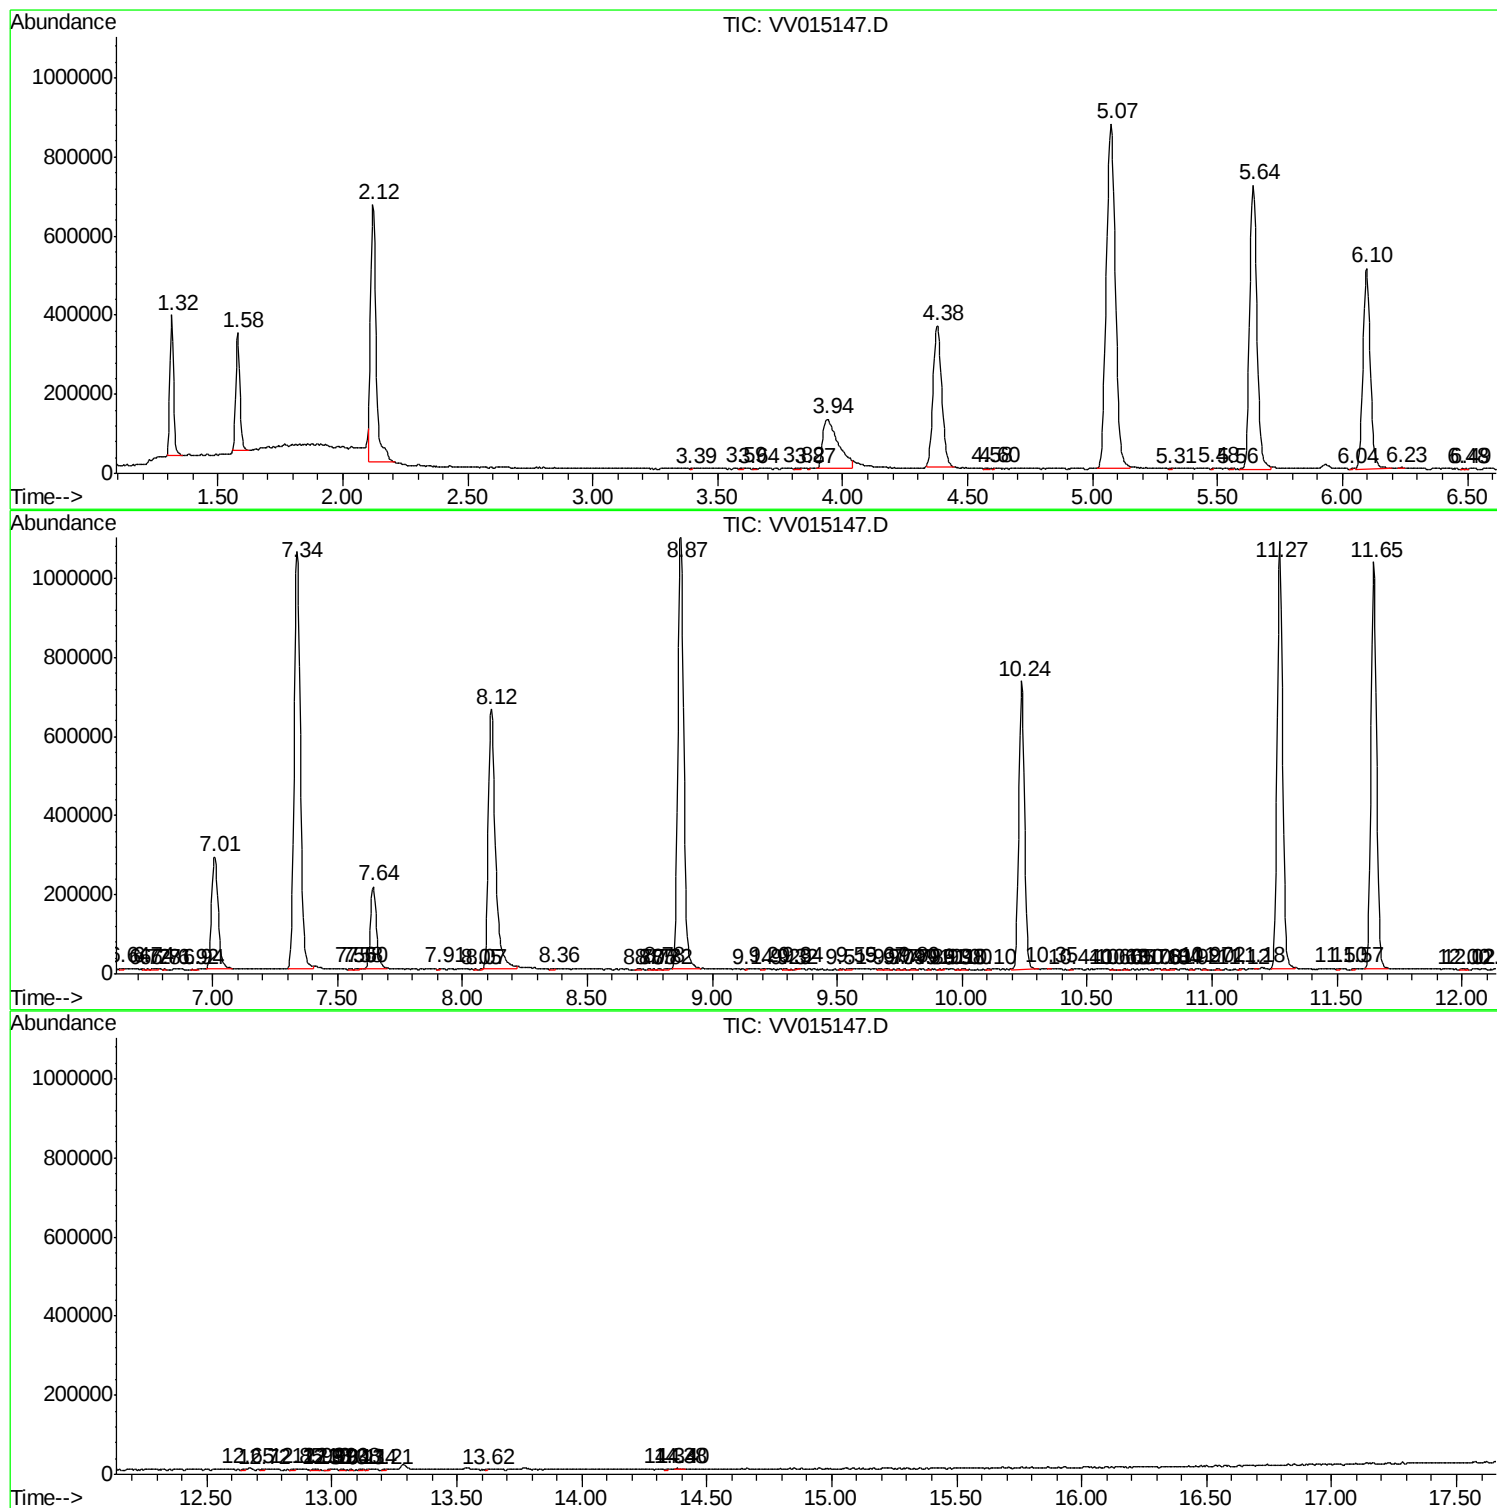

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032520\
Data File : VV015147.D
Acq On : 25 Mar 2020 20:31
Operator : SY/MD
Sample : VIBLK70
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK70

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032520\
Data File : VV015147.D
Acq On : 25 Mar 2020 20:31
Operator : SY/MD
Sample : VIBLK70
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VIBLK70

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032520WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc