

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032520\
 Data File : VV015151.D
 Acq On : 25 Mar 2020 22:08
 Operator : SY/MD
 Sample : L1968-03DL 400X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	80	rVB	351348	341957	13.75%	1.778%
2	1.579	146	152	165	rVB	301056	351530	14.14%	1.827%
3	2.119	313	320	342	rVB	674095	1028710	41.37%	5.348%
4	3.106	625	627	630	rBV3	1369	1086	0.04%	0.006%
5	3.434	724	729	732	rBV6	3024	2888	0.12%	0.015%
6	3.852	856	859	861	rBV4	1451	1040	0.04%	0.005%
7	3.939	873	886	934	rBV2	122648	573669	23.07%	2.982%
8	4.376	1010	1022	1046	rVB	355482	876331	35.24%	4.556%
9	4.662	1107	1111	1113	rBV4	2290	2039	0.08%	0.011%
10	4.749	1134	1138	1140	rBV5	1545	1011	0.04%	0.005%
11	5.074	1222	1239	1249	rBV2	890562	2215271	89.08%	11.516%
12	5.277	1298	1302	1306	rBV7	2591	2581	0.10%	0.013%
13	5.408	1340	1343	1344	rBV3	2244	1183	0.05%	0.006%
14	5.447	1352	1355	1356	rBV3	1581	824	0.03%	0.004%
15	5.486	1365	1367	1371	rBV5	3128	2476	0.10%	0.013%
16	5.643	1403	1416	1435	rBV	658967	1313009	52.80%	6.826%
17	6.096	1542	1557	1585	rBV	499054	1029890	41.41%	5.354%
18	6.428	1656	1660	1662	rBV4	2645	1916	0.08%	0.010%
19	6.559	1699	1701	1704	rBV3	1913	975	0.04%	0.005%
20	6.595	1707	1712	1716	rBV7	2116	2350	0.09%	0.012%
21	6.640	1723	1726	1729	rBV4	2530	1948	0.08%	0.010%
22	6.788	1770	1772	1774	rBV3	1685	842	0.03%	0.004%
23	6.887	1801	1803	1806	rVB4	2258	907	0.04%	0.005%
24	6.945	1818	1821	1824	rVB5	2161	1615	0.06%	0.008%
25	7.006	1825	1840	1857	rBV	288144	514562	20.69%	2.675%
26	7.251	1911	1916	1919	rBV6	1776	1657	0.07%	0.009%
27	7.293	1926	1929	1930	rBV3	1929	917	0.04%	0.005%
28	7.338	1930	1943	1967	rVV	1074052	1879949	75.60%	9.773%
29	7.643	2028	2038	2056	rBV	203634	346738	13.94%	1.802%
30	7.862	2103	2106	2107	rBV3	2806	1461	0.06%	0.008%
31	7.887	2111	2114	2117	rVV4	2424	1441	0.06%	0.007%
32	7.984	2142	2144	2146	rBV3	2054	1276	0.05%	0.007%
33	8.116	2174	2185	2208	rBV	644811	1282851	51.59%	6.669%
34	8.453	2285	2290	2291	rBV4	2248	1439	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032520\
 Data File : VV015151.D
 Acq On : 25 Mar 2020 22:08
 Operator : SY/MD
 Sample : L1968-03DL 400X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
 Title : VOC Analysis

35	8.498	2299	2304	2308	rVB7	1559	1412	0.06%	0.007%
36	8.617	2338	2341	2344	rBV5	1932	1296	0.05%	0.007%
37	8.669	2353	2357	2362	rVB8	2028	2113	0.08%	0.011%
38	8.691	2362	2364	2367	rBV3	1812	1106	0.04%	0.006%
39	8.778	2389	2391	2395	rVB4	2211	1120	0.05%	0.006%
40	8.801	2395	2398	2399	rBV2	1571	790	0.03%	0.004%
41	8.875	2405	2421	2424	rBV	1079194	1548920	62.29%	8.052%
42	9.209	2523	2525	2530	rVB6	1745	898	0.04%	0.005%
43	9.231	2530	2532	2534	rBV3	2008	879	0.04%	0.005%
44	9.283	2546	2548	2553	rVB5	2652	2068	0.08%	0.011%
45	9.312	2553	2557	2559	rBV4	2097	1259	0.05%	0.007%
46	9.392	2577	2582	2585	rBV7	1350	1229	0.05%	0.006%
47	9.457	2600	2602	2605	rVB3	1742	789	0.03%	0.004%
48	9.723	2681	2685	2687	rBV4	1479	993	0.04%	0.005%
49	9.762	2695	2697	2700	rBV4	2144	1096	0.04%	0.006%
50	9.801	2707	2709	2714	rBV5	1678	1176	0.05%	0.006%
51	9.926	2745	2748	2751	rBV6	2494	1655	0.07%	0.009%
52	9.958	2756	2758	2760	rBV3	2045	957	0.04%	0.005%
53	10.026	2775	2779	2785	rBV8	2021	2012	0.08%	0.010%
54	10.238	2832	2845	2860	rBV	723170	1128158	45.37%	5.865%
55	10.392	2891	2893	2900	rBV7	2181	1636	0.07%	0.009%
56	10.424	2900	2903	2906	rBV5	1468	1091	0.04%	0.006%
57	10.595	2951	2956	2960	rVB7	2885	2906	0.12%	0.015%
58	10.617	2960	2963	2967	rVB6	1700	1423	0.06%	0.007%
59	10.633	2967	2968	2971	rBV3	1425	775	0.03%	0.004%
60	10.720	2990	2995	2999	rBV7	1595	1617	0.07%	0.008%
61	10.759	3005	3007	3012	rVB4	1700	1066	0.04%	0.006%
62	10.794	3012	3018	3020	rBV7	2999	2487	0.10%	0.013%
63	10.868	3035	3041	3046	rBV7	3228	3932	0.16%	0.020%
64	10.907	3050	3053	3057	rVB6	2357	1633	0.07%	0.008%
65	10.932	3057	3061	3063	rBV5	2414	1649	0.07%	0.009%
66	11.026	3087	3090	3092	rBV4	1380	807	0.03%	0.004%
67	11.077	3104	3106	3111	rVB6	1676	1199	0.05%	0.006%
68	11.109	3114	3116	3119	rVB4	1626	896	0.04%	0.005%
69	11.167	3129	3134	3135	rBV5	3270	2270	0.09%	0.012%
70	11.206	3137	3146	3155	rBV2	45527	71686	2.88%	0.373%
71	11.273	3156	3167	3172	rBV	1075804	1951592	78.48%	10.145%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032520\
 Data File : VV015151.D
 Acq On : 25 Mar 2020 22:08
 Operator : SY/MD
 Sample : L1968-03DL 400X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
 Title : VOC Analysis

72	11.540	3246	3250	3252	rBV5	2187	1506	0.06%	0.008%
73	11.649	3271	3284	3306	rBV2	1193908	2486762	100.00%	12.927%
74	11.881	3352	3356	3362	rVB9	2742	2514	0.10%	0.013%
75	11.932	3370	3372	3375	rBV3	1523	883	0.04%	0.005%
76	12.196	3452	3454	3459	rBV5	1594	1161	0.05%	0.006%
77	12.321	3489	3493	3494	rBV3	2372	1308	0.05%	0.007%
78	12.553	3563	3565	3569	rVB5	2224	1318	0.05%	0.007%
79	12.579	3569	3573	3575	rBV5	2553	2156	0.09%	0.011%
80	12.662	3591	3599	3600	rBV7	4392	3881	0.16%	0.020%
81	12.765	3627	3631	3634	rBV6	1787	1606	0.06%	0.008%
82	12.810	3640	3645	3646	rBV4	1194	951	0.04%	0.005%
83	12.974	3693	3696	3699	rVB4	2817	1888	0.08%	0.010%
84	13.003	3699	3705	3706	rBV6	2645	1943	0.08%	0.010%
85	13.087	3728	3731	3737	rVB7	2573	1933	0.08%	0.010%
86	13.119	3737	3741	3743	rBV5	2113	1385	0.06%	0.007%
87	13.141	3746	3748	3753	rVV6	3009	1878	0.08%	0.010%
88	13.177	3757	3759	3763	rBV3	1490	1007	0.04%	0.005%
89	13.286	3783	3793	3805	rVB2	94110	147626	5.94%	0.767%
90	13.450	3840	3844	3846	rBV4	2710	1896	0.08%	0.010%
91	13.575	3877	3883	3887	rBV8	2240	3047	0.12%	0.016%
92	13.649	3904	3906	3909	rBV4	1660	1056	0.04%	0.005%
93	13.771	3933	3944	3952	rBV4	11608	21767	0.88%	0.113%
94	13.980	4007	4009	4012	rVB3	1942	998	0.04%	0.005%
95	14.099	4043	4046	4051	rBV7	2440	1966	0.08%	0.010%
96	14.141	4056	4059	4062	rBV5	1882	1523	0.06%	0.008%
97	14.228	4082	4086	4089	rBV5	2449	2162	0.09%	0.011%
98	14.299	4106	4108	4110	rVB3	2901	1155	0.05%	0.006%
99	14.315	4110	4113	4114	rBV3	2164	1403	0.06%	0.007%
100	14.376	4130	4132	4134	rBV3	1729	907	0.04%	0.005%


Sum of corrected areas: 19236516

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032520\
Data File : VV015151.D
Acq On : 25 Mar 2020 22:08
Operator : SY/MD
Sample : L1968-03DL 400X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DC9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

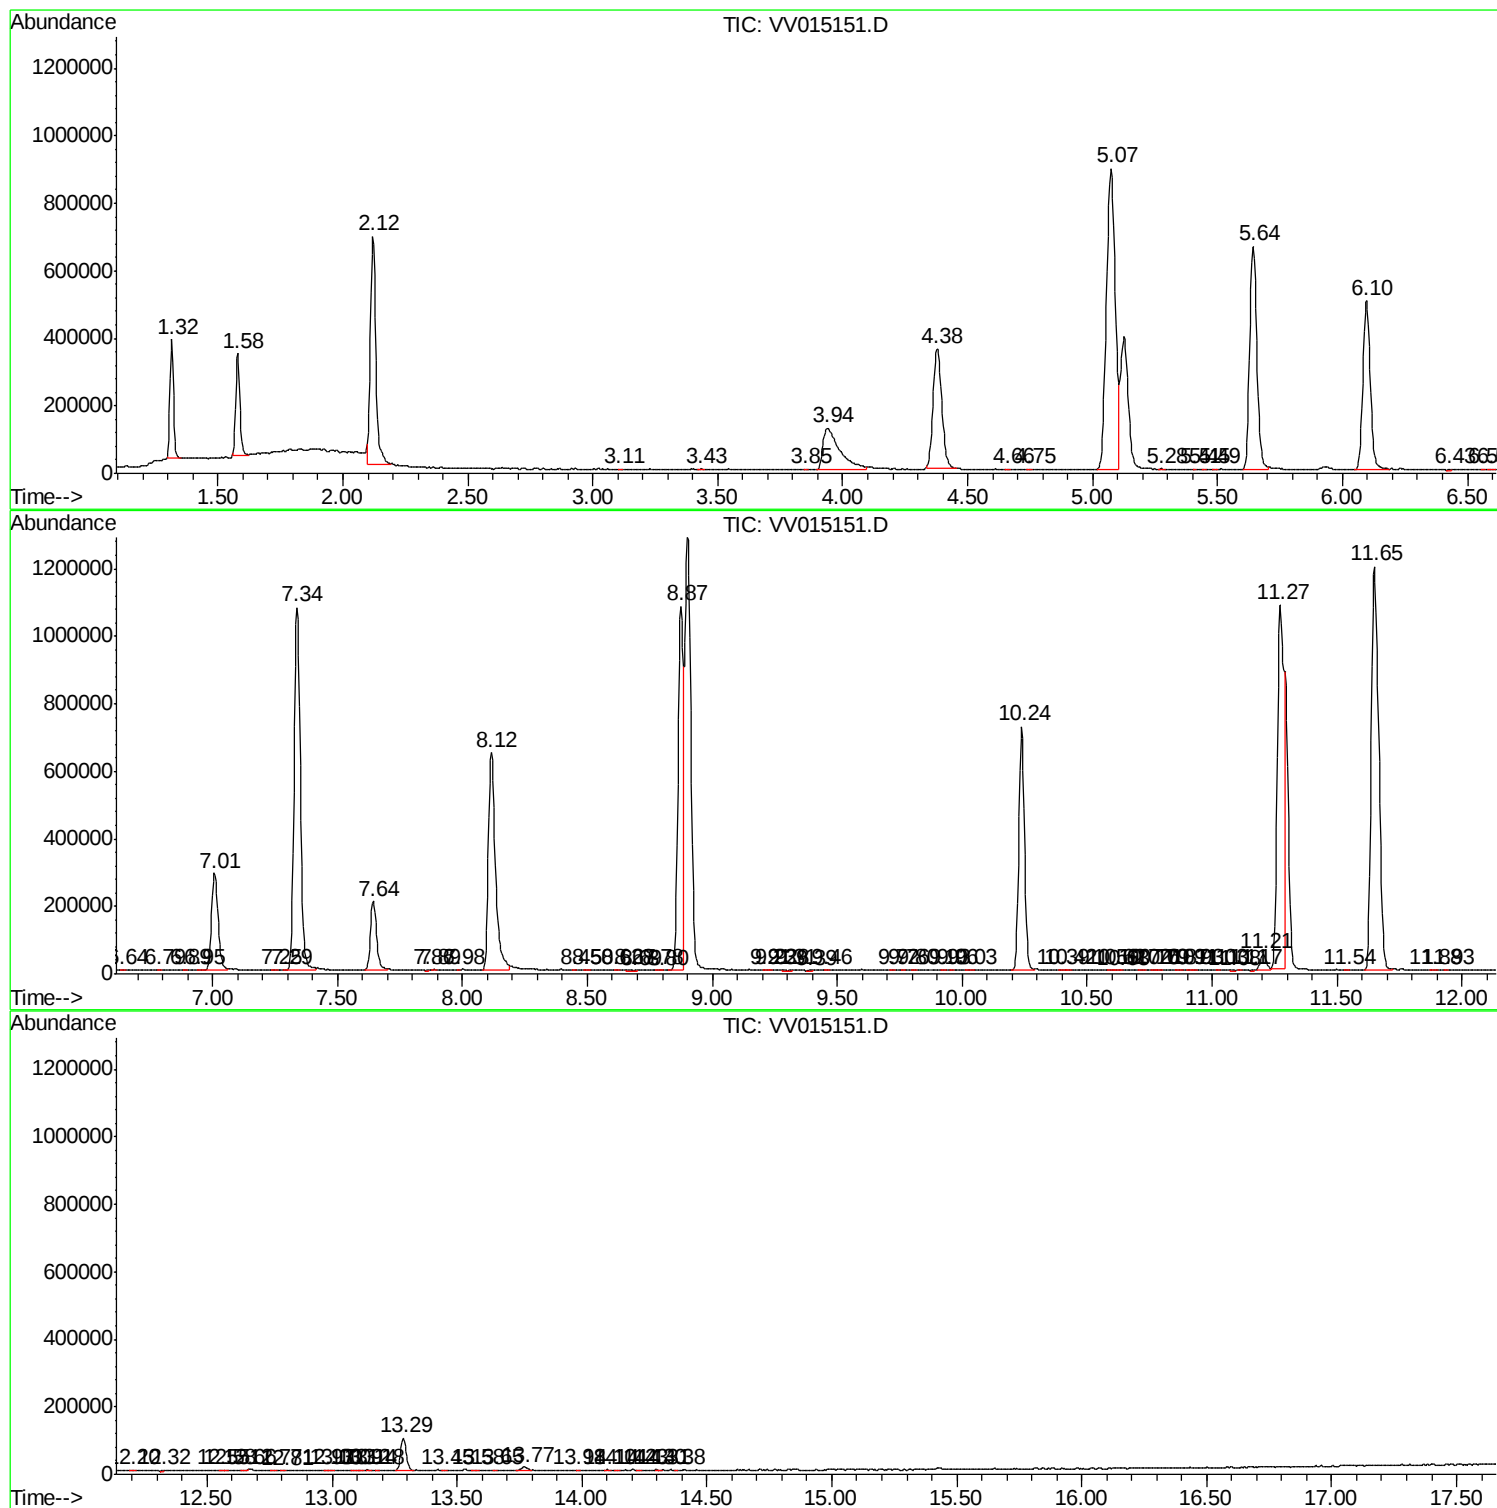

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032520\
Data File : VV015151.D
Acq On : 25 Mar 2020 22:08
Operator : SY/MD
Sample : L1968-03DL 400X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0DC9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032520WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032520\
Data File : VV015151.D
Acq On : 25 Mar 2020 22:08
Operator : SY/MD
Sample : L1968-03DL 400X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0DC9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032520WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc