

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032520\
 Data File : VV015152.D
 Acq On : 25 Mar 2020 22:32
 Operator : SY/MD
 Sample : L1968-04 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DD3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	65	70	84	rVB	340043	351648	3.32%	0.797%
2	1.579	147	152	165	rVB	298736	355186	3.35%	0.805%
3	2.119	313	320	351	rVB	690875	1115705	10.52%	2.528%
4	3.238	665	668	670	rBV4	2670	1348	0.01%	0.003%
5	3.589	774	777	778	rBV3	2157	1313	0.01%	0.003%
6	3.749	826	827	828	rBV	828	233	0.00%	0.001%
7	3.762	828	831	834	rVV5	1972	1389	0.01%	0.003%
8	3.862	860	862	863	rBV2	1210	626	0.01%	0.001%
9	3.939	874	886	929	rBV2	123168	570075	5.38%	1.292%
10	4.380	1009	1023	1041	rBV	361775	886978	8.36%	2.010%
11	4.653	1106	1108	1111	rBV4	2142	1480	0.01%	0.003%
12	4.904	1184	1186	1192	rVB7	2366	1421	0.01%	0.003%
13	5.074	1222	1239	1248	rBV2	907055	2251709	21.23%	5.102%
14	5.473	1360	1363	1365	rBV3	2705	1872	0.02%	0.004%
15	5.643	1403	1416	1439	rBV	713268	1421482	13.40%	3.221%
16	6.096	1544	1557	1580	rBV	508532	1024611	9.66%	2.322%
17	6.376	1642	1644	1651	rVB7	1524	1235	0.01%	0.003%
18	6.479	1674	1676	1681	rVB5	1314	810	0.01%	0.002%
19	6.621	1718	1720	1721	rBV2	1566	807	0.01%	0.002%
20	6.785	1767	1771	1776	rBV8	2137	2291	0.02%	0.005%
21	6.817	1779	1781	1784	rVB5	1981	990	0.01%	0.002%
22	6.875	1796	1799	1802	rVB5	1749	932	0.01%	0.002%
23	7.006	1828	1840	1859	rBV	289707	520148	4.90%	1.179%
24	7.338	1929	1943	1964	rBV	1120395	1930086	18.20%	4.374%
25	7.579	2014	2018	2020	rBV5	2008	1717	0.02%	0.004%
26	7.643	2028	2038	2062	rBV	206121	349971	3.30%	0.793%
27	7.752	2070	2072	2074	rBV3	1743	837	0.01%	0.002%
28	7.765	2074	2076	2077	rBV2	1733	802	0.01%	0.002%
29	7.910	2118	2121	2124	rBV5	1579	1051	0.01%	0.002%
30	7.955	2133	2135	2139	rVB4	2292	1061	0.01%	0.002%
31	8.061	2167	2168	2173	rBV5	1752	1067	0.01%	0.002%
32	8.116	2173	2185	2219	rBV2	639299	1305638	12.31%	2.959%
33	8.479	2294	2298	2299	rBV3	2124	1529	0.01%	0.003%
34	8.527	2311	2313	2316	rBV4	1247	617	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032520\
 Data File : VV015152.D
 Acq On : 25 Mar 2020 22:32
 Operator : SY/MD
 Sample : L1968-04 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DD3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
 Title : VOC Analysis

35	8.543	2316	2318	2320	rBV3	1496	749	0.01%	0.002%
36	8.582	2327	2330	2331	rBV3	1398	616	0.01%	0.001%
37	8.608	2336	2338	2340	rBV3	2265	1273	0.01%	0.003%
38	8.768	2386	2388	2389	rBV2	1472	618	0.01%	0.001%
39	8.797	2396	2397	2400	rVB3	1989	752	0.01%	0.002%
40	8.813	2400	2402	2405	rBV4	2260	1212	0.01%	0.003%
41	8.903	2409	2430	2455	rVV2	4088902	8322818	78.48%	18.860%
42	9.344	2560	2567	2570	rBV9	2430	2829	0.03%	0.006%
43	9.386	2578	2580	2582	rVB3	1942	852	0.01%	0.002%
44	9.408	2585	2587	2590	rBV4	990	660	0.01%	0.001%
45	9.437	2594	2596	2598	rBV3	1557	806	0.01%	0.002%
46	9.476	2605	2608	2609	rBV3	1193	753	0.01%	0.002%
47	9.598	2642	2646	2647	rBV3	2289	1401	0.01%	0.003%
48	9.637	2656	2658	2662	rBV5	1782	981	0.01%	0.002%
49	9.723	2683	2685	2686	rBV2	896	363	0.00%	0.001%
50	9.768	2698	2699	2701	rBV2	1015	477	0.00%	0.001%
51	9.807	2706	2711	2715	rVB7	2702	2914	0.03%	0.007%
52	9.836	2715	2720	2722	rBV6	2843	2078	0.02%	0.005%
53	9.846	2722	2723	2726	rBV3	1380	857	0.01%	0.002%
54	9.874	2729	2732	2733	rBV3	1384	691	0.01%	0.002%
55	9.932	2748	2750	2755	rVB6	1376	755	0.01%	0.002%
56	9.958	2756	2758	2761	rBV4	1716	1292	0.01%	0.003%
57	10.038	2777	2783	2785	rBV6	2006	2100	0.02%	0.005%
58	10.128	2809	2811	2815	rVB5	1929	1431	0.01%	0.003%
59	10.164	2819	2822	2823	rBV2	2076	1216	0.01%	0.003%
60	10.193	2827	2831	2832	rBV4	2610	1446	0.01%	0.003%
61	10.238	2834	2845	2859	rVV	746139	1146912	10.81%	2.599%
62	10.669	2974	2979	2980	rBV5	1348	1313	0.01%	0.003%
63	10.746	3001	3003	3004	rBV2	687	238	0.00%	0.001%
64	10.762	3004	3008	3009	rBV4	1844	1188	0.01%	0.003%
65	10.823	3025	3027	3028	rBV2	1118	522	0.00%	0.001%
66	10.874	3035	3043	3046	rBV8	3179	5481	0.05%	0.012%
67	10.923	3055	3058	3059	rBV3	1483	836	0.01%	0.002%
68	10.977	3073	3075	3078	rBV4	1482	656	0.01%	0.001%
69	11.013	3082	3086	3088	rBV4	2069	1431	0.01%	0.003%
70	11.080	3104	3107	3109	rBV3	1724	1037	0.01%	0.002%
71	11.145	3125	3127	3132	rVB5	2059	1207	0.01%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032520\
 Data File : VV015152.D
 Acq On : 25 Mar 2020 22:32
 Operator : SY/MD
 Sample : L1968-04 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DD3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
 Title : VOC Analysis

72	11.202	3132	3145	3156	rBV	1044163	1597080	15.06%	3.619%
73	11.292	3157	3173	3198	rVB2	4629330	8546492	80.59%	19.367%
74	11.665	3272	3289	3313	rBV2	6050985	10604963	100.00%	24.031%
75	12.157	3440	3442	3444	rBV3	2477	1425	0.01%	0.003%
76	12.212	3455	3459	3463	rBV7	3034	3039	0.03%	0.007%
77	12.296	3483	3485	3487	rBV3	1585	764	0.01%	0.002%
78	12.826	3647	3650	3652	rBV4	1463	765	0.01%	0.002%
79	12.874	3663	3665	3667	rBV3	1622	914	0.01%	0.002%
80	12.990	3698	3701	3704	rVB4	3538	2208	0.02%	0.005%
81	13.009	3704	3707	3709	rBV4	3180	1910	0.02%	0.004%
82	13.042	3714	3717	3719	rBV3	3000	1884	0.02%	0.004%
83	13.106	3735	3737	3740	rBV4	1207	608	0.01%	0.001%
84	13.138	3745	3747	3751	rBV5	1428	901	0.01%	0.002%
85	13.283	3781	3792	3813	rBV	740690	1150219	10.85%	2.606%
86	13.472	3849	3851	3855	rBV4	1919	1263	0.01%	0.003%
87	13.517	3862	3865	3866	rBV3	3002	1668	0.02%	0.004%
88	13.723	3925	3929	3931	rBV4	3339	3109	0.03%	0.007%
89	13.768	3931	3943	3963	rVB	346417	562888	5.31%	1.276%
90	15.424	4449	4458	4469	rBV	13180	26445	0.25%	0.060%


Sum of corrected areas: 44129971

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032520\
Data File : VV015152.D
Acq On : 25 Mar 2020 22:32
Operator : SY/MD
Sample : L1968-04 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0DD3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

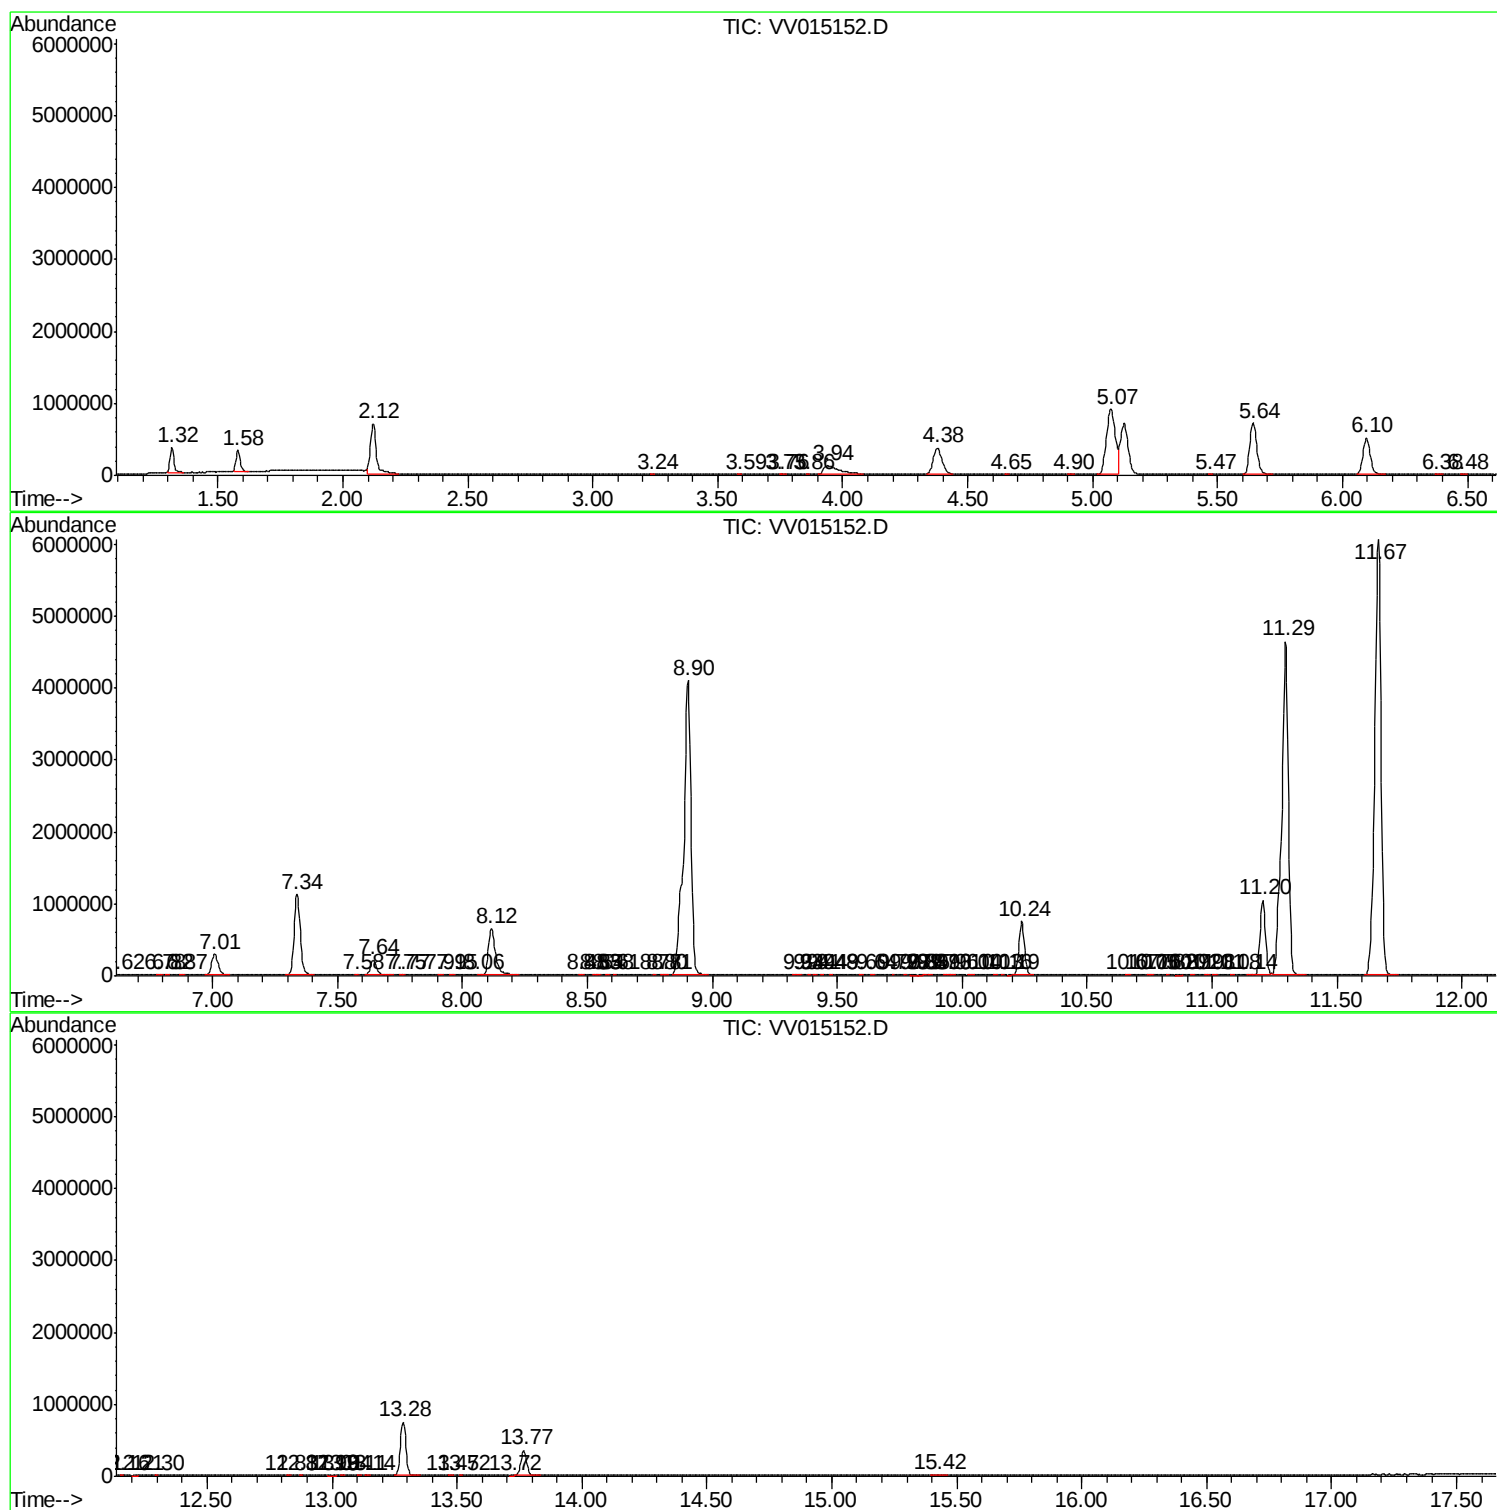

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032520\
Data File : VV015152.D
Acq On : 25 Mar 2020 22:32
Operator : SY/MD
Sample : L1968-04 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DD3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032520\
Data File : VV015152.D
Acq On : 25 Mar 2020 22:32
Operator : SY/MD
Sample : L1968-04 100X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0DD3

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032520WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc