

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032520\
 Data File : VV015156.D
 Acq On : 26 Mar 2020 00:09
 Operator : SY/MD
 Sample : L1968-12 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CODE3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB	356927	356257	4.91%	1.186%
2	1.579	146	152	166	rVB	302544	355838	4.91%	1.185%
3	2.119	313	320	333	rVB	654934	914207	12.61%	3.043%
4	3.045	604	608	613	rBV7	3941	3627	0.05%	0.012%
5	3.110	625	628	632	rVB6	1951	1429	0.02%	0.005%
6	3.187	648	652	653	rBV3	1776	1439	0.02%	0.005%
7	3.286	680	683	684	rBV3	2296	1315	0.02%	0.004%
8	3.409	717	721	723	rBV4	2381	1671	0.02%	0.006%
9	3.512	750	753	754	rBV3	1470	806	0.01%	0.003%
10	3.547	759	764	767	rBV6	2661	2888	0.04%	0.010%
11	3.717	813	817	821	rVB7	3097	1990	0.03%	0.007%
12	3.785	835	838	844	rVB7	1876	1865	0.03%	0.006%
13	3.827	848	851	854	rBV4	2091	1418	0.02%	0.005%
14	3.939	874	886	920	rBV	122138	546666	7.54%	1.820%
15	4.376	1009	1022	1047	rVB2	367424	899913	12.41%	2.996%
16	4.582	1083	1086	1089	rVB4	1994	1220	0.02%	0.004%
17	4.608	1090	1094	1096	rBV4	1807	1588	0.02%	0.005%
18	4.978	1206	1209	1213	rBV5	2504	1628	0.02%	0.005%
19	5.071	1221	1238	1250	rBV2	907555	2260028	31.18%	7.523%
20	5.376	1331	1333	1335	rBV3	1983	1236	0.02%	0.004%
21	5.483	1364	1366	1370	rBV4	1750	1313	0.02%	0.004%
22	5.531	1376	1381	1383	rBV6	1625	1507	0.02%	0.005%
23	5.563	1389	1391	1393	rBV3	1497	709	0.01%	0.002%
24	5.640	1403	1415	1436	rBV	718020	1401434	19.33%	4.665%
25	6.097	1543	1557	1583	rBV	509341	1033050	14.25%	3.439%
26	6.328	1623	1629	1633	rBV8	1577	1724	0.02%	0.006%
27	6.476	1673	1675	1681	rVB7	1599	1203	0.02%	0.004%
28	6.505	1681	1684	1688	rBV5	1941	1853	0.03%	0.006%
29	6.572	1701	1705	1708	rBV5	1473	976	0.01%	0.003%
30	6.659	1729	1732	1735	rVB5	1969	1032	0.01%	0.003%
31	6.830	1781	1785	1786	rBV4	1835	1250	0.02%	0.004%
32	7.010	1829	1841	1859	rBV	282977	511639	7.06%	1.703%
33	7.161	1884	1888	1890	rBV5	1720	1502	0.02%	0.005%
34	7.338	1928	1943	1960	rBV	1112318	1903675	26.26%	6.337%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032520\
 Data File : VV015156.D
 Acq On : 26 Mar 2020 00:09
 Operator : SY/MD
 Sample : L1968-12 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CODE3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
 Title : VOC Analysis

35	7.643	2028	2038	2054	rBV	206724	341933	4.72%	1.138%
36	7.894	2111	2116	2117	rBV4	2247	1895	0.03%	0.006%
37	8.116	2174	2185	2212	rVV	631843	1261800	17.41%	4.200%
38	8.470	2293	2295	2300	rBV5	2064	1377	0.02%	0.005%
39	8.492	2300	2302	2305	rBV4	2329	1557	0.02%	0.005%
40	8.643	2347	2349	2352	rBV4	1664	1062	0.01%	0.004%
41	8.720	2369	2373	2377	rBV7	2814	2129	0.03%	0.007%
42	8.775	2385	2390	2394	rVB7	1813	1521	0.02%	0.005%
43	8.875	2409	2421	2424	rBV	1165302	1684983	23.24%	5.609%
44	9.100	2489	2491	2495	rBV5	1815	1211	0.02%	0.004%
45	9.154	2504	2508	2511	rBV6	3472	3177	0.04%	0.011%
46	9.199	2519	2522	2526	rBV4	2050	1726	0.02%	0.006%
47	9.351	2567	2569	2571	rBV3	1669	1017	0.01%	0.003%
48	9.437	2593	2596	2598	rVB3	1478	893	0.01%	0.003%
49	9.453	2598	2601	2603	rBV4	1540	1223	0.02%	0.004%
50	9.662	2659	2666	2667	rBV7	2899	2770	0.04%	0.009%
51	9.707	2677	2680	2682	rVB3	1494	845	0.01%	0.003%
52	9.817	2710	2714	2715	rBV4	1817	1162	0.02%	0.004%
53	9.920	2743	2746	2748	rBV4	1845	1150	0.02%	0.004%
54	9.955	2752	2757	2760	rBV7	2782	2294	0.03%	0.008%
55	10.032	2778	2781	2784	rBV4	1080	725	0.01%	0.002%
56	10.064	2786	2791	2793	rBV6	1137	1212	0.02%	0.004%
57	10.164	2820	2822	2824	rBV3	1737	1194	0.02%	0.004%
58	10.190	2828	2830	2833	rVV4	1038	810	0.01%	0.003%
59	10.238	2833	2845	2861	rVV	743087	1147414	15.83%	3.820%
60	10.334	2873	2875	2877	rBV3	1512	782	0.01%	0.003%
61	10.405	2894	2897	2900	rBV5	1445	1219	0.02%	0.004%
62	10.450	2907	2911	2915	rBV6	2867	2377	0.03%	0.008%
63	10.514	2925	2931	2934	rBV8	1477	1417	0.02%	0.005%
64	10.531	2934	2936	2939	rBV3	2736	1797	0.02%	0.006%
65	10.559	2943	2945	2947	rBV4	2769	1797	0.02%	0.006%
66	10.682	2978	2983	2988	rBV9	1678	1865	0.03%	0.006%
67	10.707	2988	2991	2994	rBV5	2050	1321	0.02%	0.004%
68	10.801	3015	3020	3025	rBV8	1752	1449	0.02%	0.005%
69	10.987	3076	3078	3081	rVB4	1708	801	0.01%	0.003%
70	11.003	3081	3083	3088	rVB5	3049	2153	0.03%	0.007%
71	11.035	3088	3093	3095	rBV5	3354	3217	0.04%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032520\
 Data File : VV015156.D
 Acq On : 26 Mar 2020 00:09
 Operator : SY/MD
 Sample : L1968-12 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CODE3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
 Title : VOC Analysis

72	11.119	3116	3119	3120	rBV3	2442	1561	0.02%	0.005%
73	11.203	3132	3145	3156	rBV	821214	1248871	17.23%	4.157%
74	11.293	3156	3173	3194	rVB2	2438563	5210703	71.88%	17.346%
75	11.666	3267	3289	3307	rBV2	3820674	7249205	100.00%	24.132%
76	12.077	3412	3417	3420	rBV6	2160	2144	0.03%	0.007%
77	12.148	3436	3439	3440	rBV3	1401	669	0.01%	0.002%
78	12.241	3466	3468	3471	rVB4	1402	716	0.01%	0.002%
79	12.267	3473	3476	3478	rBV3	2047	1619	0.02%	0.005%
80	12.331	3492	3496	3498	rBV4	1818	1316	0.02%	0.004%
81	12.344	3498	3500	3507	rVB7	1656	1606	0.02%	0.005%
82	12.373	3507	3509	3514	rVB6	2009	1881	0.03%	0.006%
83	12.399	3514	3517	3519	rBV4	2991	2565	0.04%	0.009%
84	12.479	3539	3542	3545	rBV5	1320	1113	0.02%	0.004%
85	12.669	3592	3601	3610	rVB5	5237	10246	0.14%	0.034%
86	12.711	3610	3614	3615	rBV4	2896	2004	0.03%	0.007%
87	12.817	3644	3647	3650	rVB4	3693	2196	0.03%	0.007%
88	12.836	3650	3653	3654	rBV3	2833	1471	0.02%	0.005%
89	12.878	3663	3666	3668	rBV4	2204	1401	0.02%	0.005%
90	12.920	3675	3679	3681	rBV5	1947	1298	0.02%	0.004%
91	13.010	3705	3707	3709	rBV3	1694	792	0.01%	0.003%
92	13.112	3736	3739	3741	rBV4	1996	1447	0.02%	0.005%
93	13.222	3771	3773	3775	rBV3	1848	1098	0.02%	0.004%
94	13.286	3781	3793	3812	rBV	623350	964783	13.31%	3.212%
95	13.450	3842	3844	3845	rBV2	1733	716	0.01%	0.002%
96	13.669	3904	3912	3915	rBV8	2706	4218	0.06%	0.014%
97	13.707	3920	3924	3927	rVV6	2317	1905	0.03%	0.006%
98	13.768	3932	3943	3957	rVV	390553	612362	8.45%	2.038%
99	14.064	4032	4035	4038	rBV4	2262	1916	0.03%	0.006%
100	14.247	4090	4092	4096	rVB5	1593	900	0.01%	0.003%


Sum of corrected areas: 30039893

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032520\
Data File : VV015156.D
Acq On : 26 Mar 2020 00:09
Operator : SY/MD
Sample : L1968-12 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CODE3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

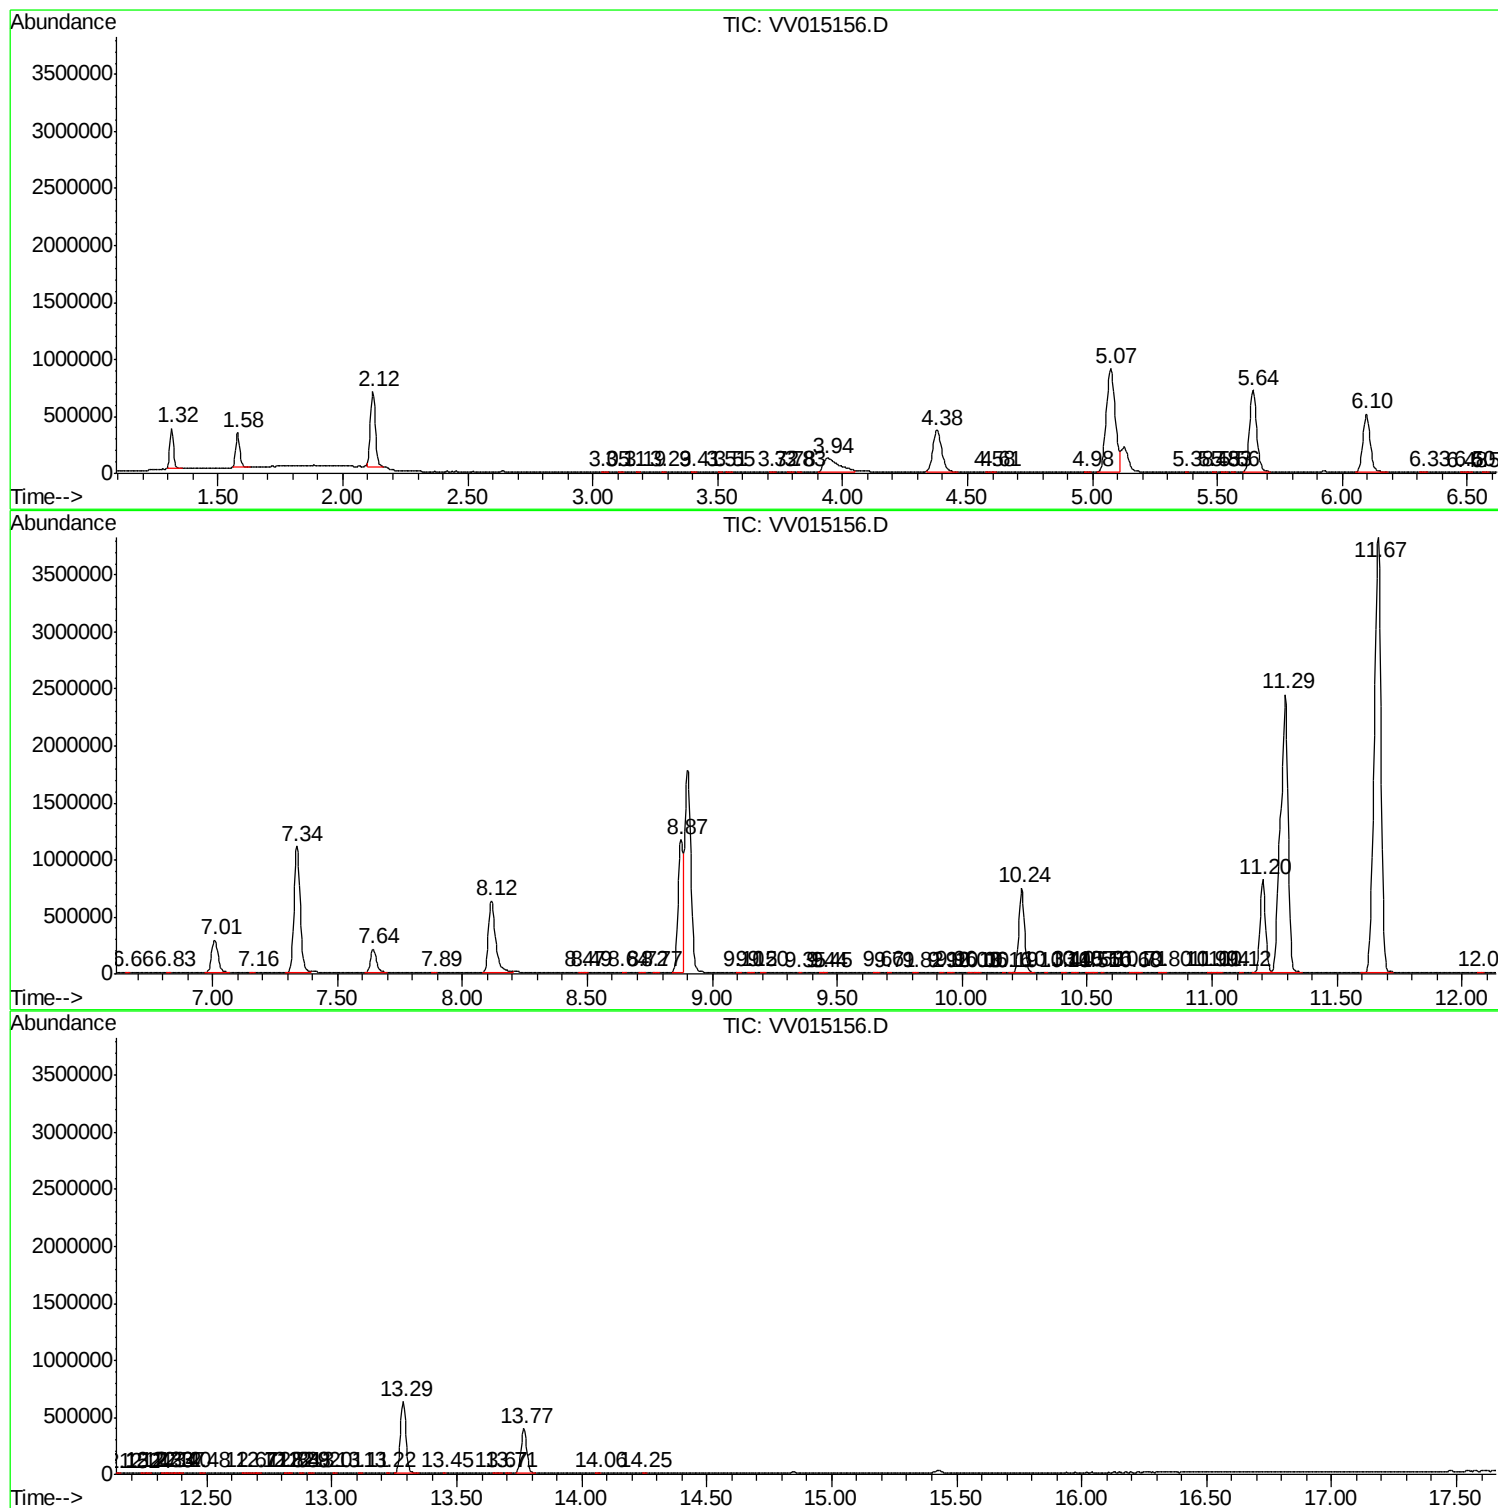

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032520\
Data File : VV015156.D
Acq On : 26 Mar 2020 00:09
Operator : SY/MD
Sample : L1968-12 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CODE3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032520\
Data File : VV015156.D
Acq On : 26 Mar 2020 00:09
Operator : SY/MD
Sample : L1968-12 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DE3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc