

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032520\
 Data File : VV015158.D
 Acq On : 26 Mar 2020 00:58
 Operator : SY/MD
 Sample : L1968-13DL 1000X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CODE5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	335139	333600	13.24%	1.720%
2	1.579	146	152	163	rBV	285344	333197	13.22%	1.718%
3	2.119	313	320	333	rVB	615869	863346	34.27%	4.452%
4	3.248	667	671	673	rBV5	3174	2571	0.10%	0.013%
5	3.396	715	717	721	rBV5	2113	1211	0.05%	0.006%
6	3.560	764	768	771	rBV4	2322	2412	0.10%	0.012%
7	3.701	809	812	815	rBV5	2296	1952	0.08%	0.010%
8	3.746	824	826	830	rVB5	2105	1350	0.05%	0.007%
9	3.762	830	831	834	rBV3	1526	1063	0.04%	0.005%
10	3.833	851	853	855	rBV3	1689	933	0.04%	0.005%
11	3.939	874	886	931	rBV	121684	562642	22.33%	2.901%
12	4.280	989	992	997	rBV6	2636	2787	0.11%	0.014%
13	4.309	997	1001	1003	rBV5	2346	1885	0.07%	0.010%
14	4.376	1009	1022	1047	rVB	350553	870383	34.55%	4.488%
15	4.724	1127	1130	1133	rBV5	2506	1649	0.07%	0.009%
16	5.074	1221	1239	1251	rBV2	872251	2205894	87.55%	11.374%
17	5.341	1319	1322	1323	rBV3	2274	1295	0.05%	0.007%
18	5.640	1402	1415	1440	rBV	676724	1350119	53.59%	6.962%
19	5.991	1520	1524	1532	rVB9	2690	3356	0.13%	0.017%
20	6.097	1544	1557	1580	rBV	489122	984975	39.09%	5.079%
21	6.508	1682	1685	1686	rBV2	1841	967	0.04%	0.005%
22	6.566	1700	1703	1707	rBV5	1369	1163	0.05%	0.006%
23	6.589	1707	1710	1713	rVB5	2793	1966	0.08%	0.010%
24	6.611	1713	1717	1720	rBV5	2095	1576	0.06%	0.008%
25	6.634	1720	1724	1725	rBV4	2844	2170	0.09%	0.011%
26	6.656	1729	1731	1734	rVB4	1781	993	0.04%	0.005%
27	6.769	1762	1766	1767	rBV4	1397	933	0.04%	0.005%
28	6.782	1767	1770	1773	rVB4	1565	885	0.04%	0.005%
29	6.865	1791	1796	1800	rVB6	3523	2613	0.10%	0.013%
30	6.891	1800	1804	1806	rBV5	1676	1455	0.06%	0.008%
31	6.939	1812	1819	1820	rBV6	1824	1847	0.07%	0.010%
32	7.010	1826	1841	1856	rBV	275185	499430	19.82%	2.575%
33	7.338	1931	1943	1959	rBV	1046110	1799540	71.42%	9.279%
34	7.643	2028	2038	2054	rBV	196008	330507	13.12%	1.704%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032520\
 Data File : VV015158.D
 Acq On : 26 Mar 2020 00:58
 Operator : SY/MD
 Sample : L1968-13DL 1000X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CODE5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
 Title : VOC Analysis

35	7.904	2116	2119	2121	rBV4	1713	1208	0.05%	0.006%
36	7.955	2132	2135	2139	rBV6	2053	1954	0.08%	0.010%
37	8.116	2175	2185	2210	rBV	621496	1237709	49.12%	6.382%
38	8.367	2261	2263	2265	rBV2	1914	1038	0.04%	0.005%
39	8.473	2291	2296	2302	rBV9	3324	4219	0.17%	0.022%
40	8.534	2312	2315	2319	rBV5	1728	1179	0.05%	0.006%
41	8.556	2319	2322	2324	rBV4	1926	1184	0.05%	0.006%
42	8.595	2330	2334	2335	rBV3	2029	1382	0.05%	0.007%
43	8.830	2405	2407	2408	rBV2	1856	820	0.03%	0.004%
44	8.875	2409	2421	2425	rBV	1112810	1735704	68.89%	8.950%
45	9.129	2497	2500	2501	rBV3	1765	845	0.03%	0.004%
46	9.158	2506	2509	2514	rBV7	3042	3451	0.14%	0.018%
47	9.264	2539	2542	2546	rBV6	2088	1567	0.06%	0.008%
48	9.379	2574	2578	2580	rBV4	2037	1280	0.05%	0.007%
49	9.402	2580	2585	2591	rVB10	2453	2205	0.09%	0.011%
50	9.428	2591	2593	2599	rVB5	2499	2248	0.09%	0.012%
51	9.466	2602	2605	2610	rVB7	2341	2112	0.08%	0.011%
52	9.489	2610	2612	2616	rBV4	1996	1148	0.05%	0.006%
53	9.511	2616	2619	2624	rBV6	2000	1758	0.07%	0.009%
54	9.534	2624	2626	2628	rBV3	1796	1054	0.04%	0.005%
55	9.695	2671	2676	2678	rBV6	1479	1412	0.06%	0.007%
56	9.746	2689	2692	2694	rBV4	1544	1055	0.04%	0.005%
57	9.785	2699	2704	2708	rBV7	1800	1768	0.07%	0.009%
58	10.090	2793	2799	2806	rBV10	3437	3756	0.15%	0.019%
59	10.164	2820	2822	2827	rVB5	1805	852	0.03%	0.004%
60	10.238	2833	2845	2863	rBV	710219	1114457	44.23%	5.747%
61	10.447	2909	2910	2914	rVB4	1721	1073	0.04%	0.006%
62	10.476	2914	2919	2925	rVB10	2027	2444	0.10%	0.013%
63	10.563	2938	2946	2948	rBV8	2895	2894	0.11%	0.015%
64	10.640	2966	2970	2976	rBV8	2253	2911	0.12%	0.015%
65	10.666	2976	2978	2984	rVB6	2468	1617	0.06%	0.008%
66	10.695	2984	2987	2993	rBV7	1881	1852	0.07%	0.010%
67	10.730	2995	2998	3003	rBV7	2082	2029	0.08%	0.010%
68	10.807	3019	3022	3025	rBV4	1218	968	0.04%	0.005%
69	10.859	3029	3038	3041	rBV4	2895	3753	0.15%	0.019%
70	10.875	3041	3043	3048	rVB5	2583	1778	0.07%	0.009%
71	10.926	3056	3059	3061	rBV4	1418	841	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032520\
 Data File : VV015158.D
 Acq On : 26 Mar 2020 00:58
 Operator : SY/MD
 Sample : L1968-13DL 1000X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CODE5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
 Title : VOC Analysis

72	10.977	3072	3075	3080	rVB6	2387	1631	0.06%	0.008%
73	11.006	3080	3084	3087	rBV5	1628	1401	0.06%	0.007%
74	11.055	3097	3099	3102	rVB4	2464	1536	0.06%	0.008%
75	11.145	3125	3127	3131	rVB5	1953	1079	0.04%	0.006%
76	11.203	3132	3145	3155	rBV	49125	87113	3.46%	0.449%
77	11.270	3155	3166	3189	rVV2	1069930	2172169	86.21%	11.200%
78	11.650	3271	3284	3305	rBV2	1172055	2519535	100.00%	12.992%
79	11.997	3384	3392	3396	rBV10	2423	2975	0.12%	0.015%
80	12.064	3410	3413	3415	rBV4	1853	968	0.04%	0.005%
81	12.113	3426	3428	3429	rBV2	2179	1021	0.04%	0.005%
82	12.363	3503	3506	3510	rBV7	2610	1652	0.07%	0.009%
83	12.412	3516	3521	3525	rBV8	2551	2692	0.11%	0.014%
84	12.457	3531	3535	3538	rBV6	1837	1739	0.07%	0.009%
85	12.489	3543	3545	3550	rVB5	1831	1168	0.05%	0.006%
86	12.514	3550	3553	3555	rBV4	1956	1299	0.05%	0.007%
87	12.730	3617	3620	3624	rVB6	1763	1377	0.05%	0.007%
88	12.778	3632	3635	3639	rBV4	2361	2383	0.09%	0.012%
89	12.830	3648	3651	3654	rVB5	1420	988	0.04%	0.005%
90	12.852	3654	3658	3660	rBV5	2060	1650	0.07%	0.009%
91	13.138	3741	3747	3748	rBV6	2122	1898	0.08%	0.010%
92	13.190	3760	3763	3765	rBV3	2583	1482	0.06%	0.008%
93	13.286	3782	3793	3807	rBV	122442	191644	7.61%	0.988%
94	13.415	3829	3833	3835	rBV5	1469	1270	0.05%	0.007%
95	13.521	3862	3866	3867	rBV3	2808	1978	0.08%	0.010%
96	13.620	3894	3897	3899	rBV4	1542	983	0.04%	0.005%
97	13.768	3935	3943	3955	rVB4	37868	61516	2.44%	0.317%
98	13.858	3968	3971	3975	rBV5	2870	2852	0.11%	0.015%
99	13.961	3998	4003	4006	rBV7	3157	2484	0.10%	0.013%
100	14.061	4032	4034	4036	rBV3	1955	986	0.04%	0.005%


Sum of corrected areas: 19393659

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032520\
Data File : VV015158.D
Acq On : 26 Mar 2020 00:58
Operator : SY/MD
Sample : L1968-13DL 1000X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DE5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

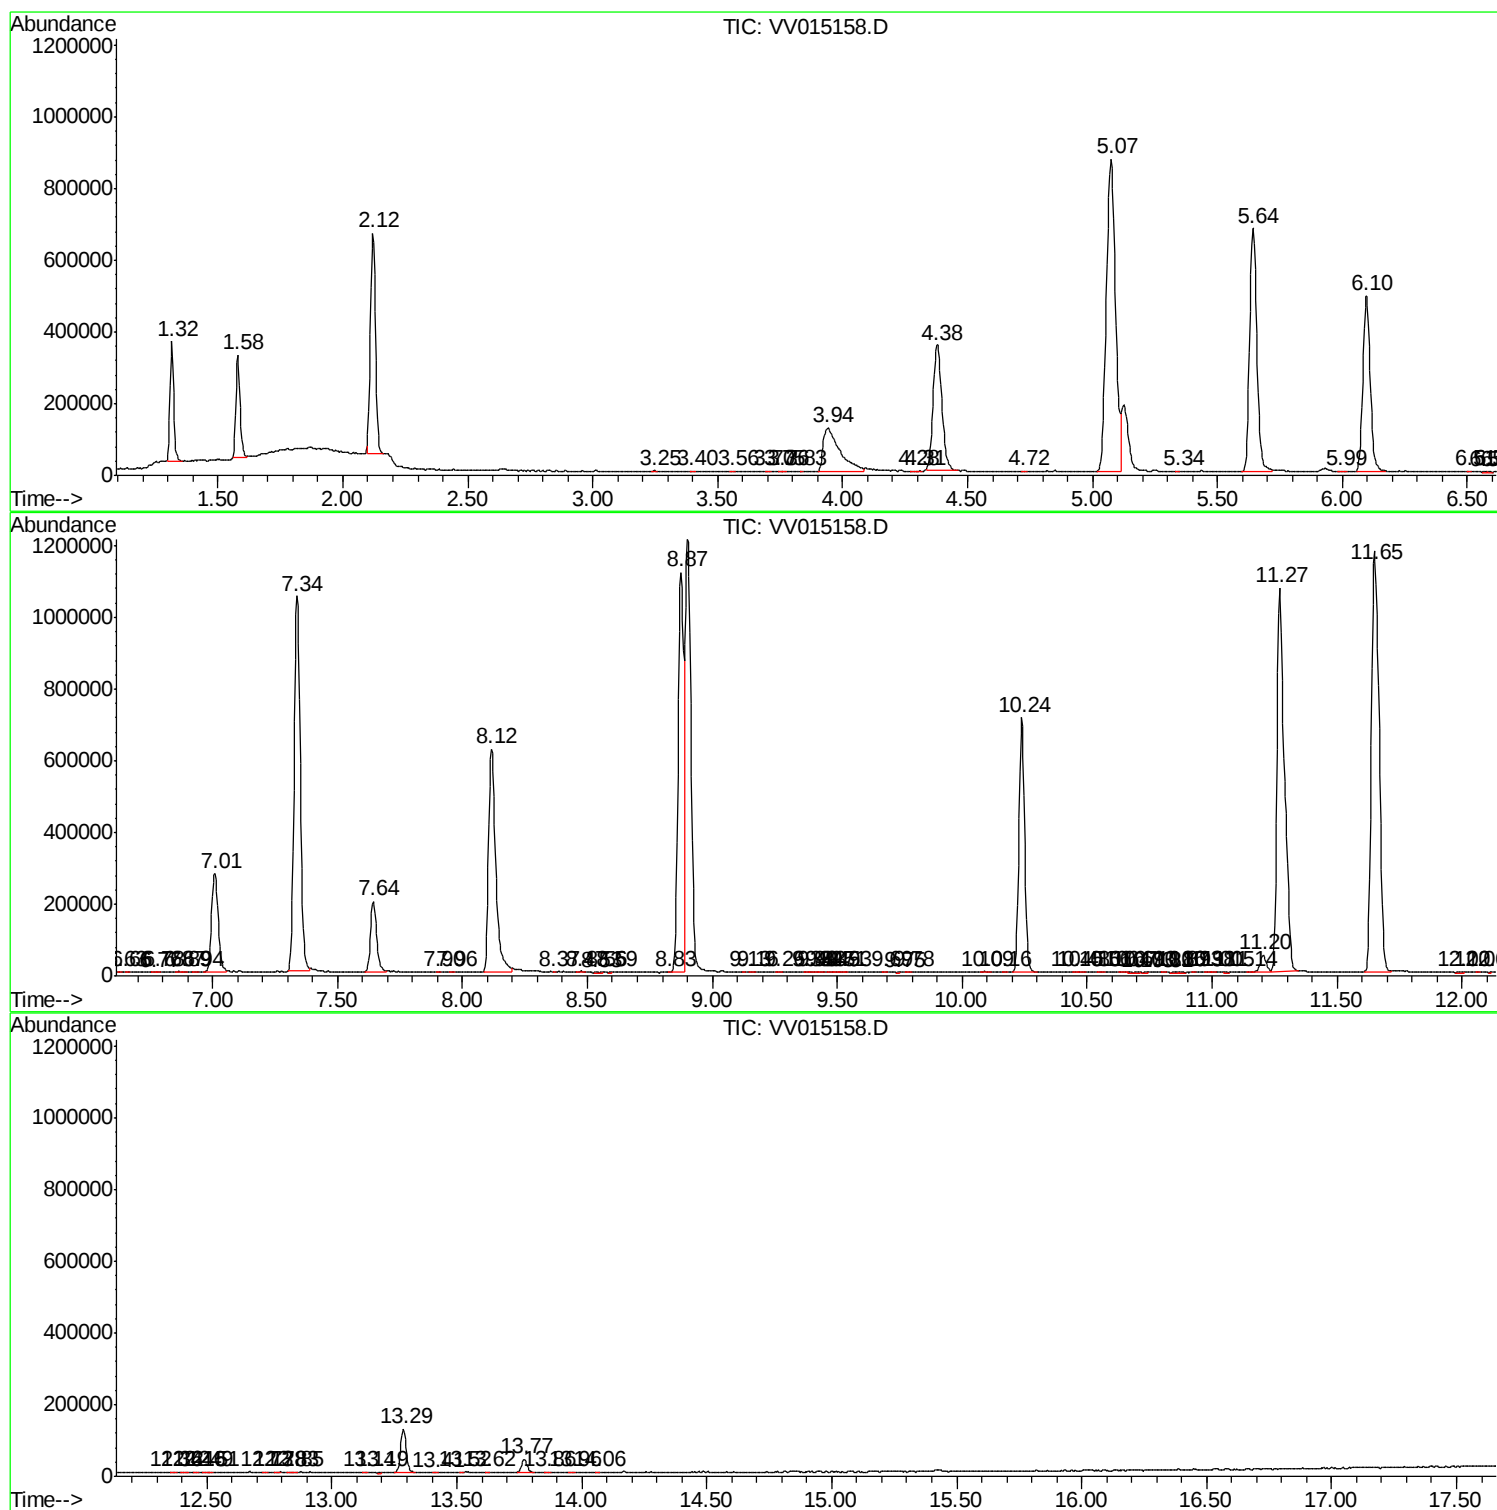

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032520\
Data File : VV015158.D
Acq On : 26 Mar 2020 00:58
Operator : SY/MD
Sample : L1968-13DL 1000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DE5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032520\
Data File : VV015158.D
Acq On : 26 Mar 2020 00:58
Operator : SY/MD
Sample : L1968-13DL 1000X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0DE5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032520WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc