

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032520\
 Data File : VV015159.D
 Acq On : 26 Mar 2020 01:22
 Operator : SY/MD
 Sample : L1968-14 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DF1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	81	rVB	330833	341729	1.32%	0.580%
2	1.579	146	152	165	rVB	301027	356845	1.37%	0.605%
3	2.119	313	320	342	rVB	683610	1044877	4.02%	1.773%
4	3.206	656	658	661	rVB3	2126	1013	0.00%	0.002%
5	3.338	697	699	704	rVB6	1734	1236	0.00%	0.002%
6	3.377	708	711	714	rBV5	1449	1345	0.01%	0.002%
7	3.454	732	735	736	rBV3	1318	735	0.00%	0.001%
8	3.701	809	812	817	rVB6	2176	1931	0.01%	0.003%
9	3.939	874	886	925	rBV	118373	556972	2.14%	0.945%
10	4.376	1009	1022	1045	rVB	355431	872184	3.36%	1.480%
11	4.653	1105	1108	1112	rBV5	2223	1581	0.01%	0.003%
12	4.676	1112	1115	1120	rBV7	2542	2790	0.01%	0.005%
13	4.839	1162	1166	1167	rBV3	2218	1676	0.01%	0.003%
14	5.071	1222	1238	1275	rBV2	892195	2364103	9.10%	4.011%
15	5.322	1314	1316	1318	rBV3	1500	513	0.00%	0.001%
16	5.640	1398	1415	1441	rBV	719349	1437881	5.54%	2.439%
17	6.007	1524	1529	1530	rBV5	2010	1546	0.01%	0.003%
18	6.093	1543	1556	1579	rBV3	508449	1023408	3.94%	1.736%
19	6.431	1654	1661	1664	rBV8	1677	2226	0.01%	0.004%
20	6.515	1685	1687	1689	rBV3	1461	853	0.00%	0.001%
21	6.547	1694	1697	1700	rVB5	1261	895	0.00%	0.002%
22	6.598	1711	1713	1715	rBV3	1502	746	0.00%	0.001%
23	6.753	1758	1761	1762	rBV3	2451	1365	0.01%	0.002%
24	6.814	1778	1780	1784	rVB5	1806	1307	0.01%	0.002%
25	6.839	1784	1788	1795	rVB9	2250	2148	0.01%	0.004%
26	6.868	1795	1797	1800	rBV3	1719	1330	0.01%	0.002%
27	6.920	1810	1813	1816	rBV5	1802	1199	0.00%	0.002%
28	6.965	1823	1827	1828	rBV4	1699	954	0.00%	0.002%
29	7.007	1829	1840	1856	rVV	282080	513146	1.98%	0.871%
30	7.338	1930	1943	1966	rBV	1099609	1907004	7.34%	3.235%
31	7.585	2017	2020	2026	rVB7	2366	2375	0.01%	0.004%
32	7.643	2026	2038	2056	rBV	201720	355523	1.37%	0.603%
33	8.116	2174	2185	2216	rBV2	627935	1265913	4.87%	2.148%
34	8.450	2286	2289	2292	rBV4	2426	2040	0.01%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032520\
 Data File : VV015159.D
 Acq On : 26 Mar 2020 01:22
 Operator : SY/MD
 Sample : L1968-14 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DF1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
 Title : VOC Analysis

35	8.521	2309	2311	2314	rVB4	2354	1192	0.00%	0.002%
36	8.547	2314	2319	2321	rBV7	2589	2753	0.01%	0.005%
37	8.595	2333	2334	2337	rBV3	996	532	0.00%	0.001%
38	8.624	2340	2343	2347	rVB5	2001	1659	0.01%	0.003%
39	8.640	2347	2348	2351	rBV3	1062	575	0.00%	0.001%
40	8.717	2369	2372	2374	rBV3	1381	732	0.00%	0.001%
41	8.730	2374	2376	2378	rVV3	1457	661	0.00%	0.001%
42	8.759	2382	2385	2390	rVB7	2340	1709	0.01%	0.003%
43	8.785	2390	2393	2395	rBV3	2821	1984	0.01%	0.003%
44	8.904	2408	2430	2462	rBV	15262414	25977840	100.00%	44.070%
45	9.363	2569	2573	2577	rVB6	1807	1840	0.01%	0.003%
46	9.428	2590	2593	2594	rBV3	1338	733	0.00%	0.001%
47	9.759	2694	2696	2698	rBV3	1311	752	0.00%	0.001%
48	9.801	2708	2709	2711	rBV2	1765	883	0.00%	0.001%
49	9.839	2717	2721	2726	rBV8	1763	1605	0.01%	0.003%
50	9.926	2746	2748	2751	rBV3	1424	788	0.00%	0.001%
51	9.961	2756	2759	2760	rBV3	1760	1020	0.00%	0.002%
52	10.032	2778	2781	2783	rBV5	1586	718	0.00%	0.001%
53	10.051	2783	2787	2788	rBV4	1513	852	0.00%	0.001%
54	10.090	2796	2799	2801	rBV3	1987	1543	0.01%	0.003%
55	10.238	2827	2845	2860	rBV	739120	1151569	4.43%	1.954%
56	10.373	2886	2887	2890	rBV3	1250	651	0.00%	0.001%
57	10.418	2894	2901	2903	rBV7	2146	2481	0.01%	0.004%
58	10.444	2904	2909	2913	rBV8	3478	3231	0.01%	0.005%
59	10.547	2939	2941	2943	rBV3	2708	1368	0.01%	0.002%
60	10.588	2952	2954	2955	rBV2	1337	594	0.00%	0.001%
61	10.643	2969	2971	2976	rVB4	1357	965	0.00%	0.002%
62	10.688	2982	2985	2987	rBV3	1278	841	0.00%	0.001%
63	10.765	3004	3009	3015	rBV8	1598	1883	0.01%	0.003%
64	10.836	3025	3031	3032	rBV6	1496	1601	0.01%	0.003%
65	10.913	3052	3055	3058	rBV5	1889	882	0.00%	0.001%
66	10.958	3067	3069	3073	rVB5	2405	1619	0.01%	0.003%
67	10.990	3073	3079	3083	rBV8	2428	2863	0.01%	0.005%
68	11.064	3099	3102	3104	rBV3	1155	552	0.00%	0.001%
69	11.090	3107	3110	3112	rBV4	1932	903	0.00%	0.002%
70	11.141	3124	3126	3128	rBV3	1036	687	0.00%	0.001%
71	11.161	3130	3132	3134	rVV3	1399	797	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032520\
 Data File : VV015159.D
 Acq On : 26 Mar 2020 01:22
 Operator : SY/MD
 Sample : L1968-14 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DF1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
 Title : VOC Analysis

72	11.203	3134	3145	3156	rVV	822026	1239526	4.77%	2.103%
73	11.293	3156	3173	3199	rVB2	3766847	7312751	28.15%	12.406%
74	11.450	3220	3222	3225	rBV4	2212	1552	0.01%	0.003%
75	11.666	3267	3289	3310	rBV2	6011454	10586346	40.75%	17.959%
76	12.116	3427	3429	3431	rBV3	1179	511	0.00%	0.001%
77	12.132	3431	3434	3435	rBV3	1551	954	0.00%	0.002%
78	12.199	3453	3455	3458	rBV3	1320	951	0.00%	0.002%
79	12.244	3467	3469	3471	rVB3	1655	538	0.00%	0.001%
80	12.257	3471	3473	3478	rBV4	1869	1166	0.00%	0.002%
81	12.299	3482	3486	3487	rBV4	2329	1623	0.01%	0.003%
82	12.341	3496	3499	3500	rBV3	1737	1110	0.00%	0.002%
83	12.485	3540	3544	3547	rBV7	1771	1580	0.01%	0.003%
84	12.936	3681	3684	3691	rBV9	2839	2854	0.01%	0.005%
85	12.971	3692	3695	3700	rVV6	2226	1497	0.01%	0.003%
86	13.286	3782	3793	3810	rVB	285695	455603	1.75%	0.773%
87	13.350	3811	3813	3816	rBV4	2008	1046	0.00%	0.002%
88	13.437	3837	3840	3845	rBV6	2744	2712	0.01%	0.005%
89	13.617	3894	3896	3899	rVB4	2403	1257	0.00%	0.002%
90	13.633	3899	3901	3902	rBV2	1287	536	0.00%	0.001%
91	13.688	3915	3918	3922	rBV7	2103	1472	0.01%	0.002%
92	13.768	3932	3943	3954	rBV2	39817	67386	0.26%	0.114%
93	13.855	3967	3970	3976	rVB8	2549	2491	0.01%	0.004%
94	13.884	3976	3979	3981	rBV4	2284	1571	0.01%	0.003%
95	13.926	3990	3992	3994	rBV3	1769	916	0.00%	0.002%
96	13.939	3994	3996	4000	rVV4	2590	1326	0.01%	0.002%
97	14.035	4022	4026	4033	rBV9	2035	3242	0.01%	0.005%
98	14.563	4187	4190	4193	rBV4	1755	1038	0.00%	0.002%
99	14.823	4269	4271	4274	rBV3	2725	1558	0.01%	0.003%
100	14.849	4274	4279	4286	rVB9	5954	6591	0.03%	0.011%




Sum of corrected areas: 58946951

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032520\
Data File : VV015159.D
Acq On : 26 Mar 2020 01:22
Operator : SY/MD
Sample : L1968-14 200X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DF1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

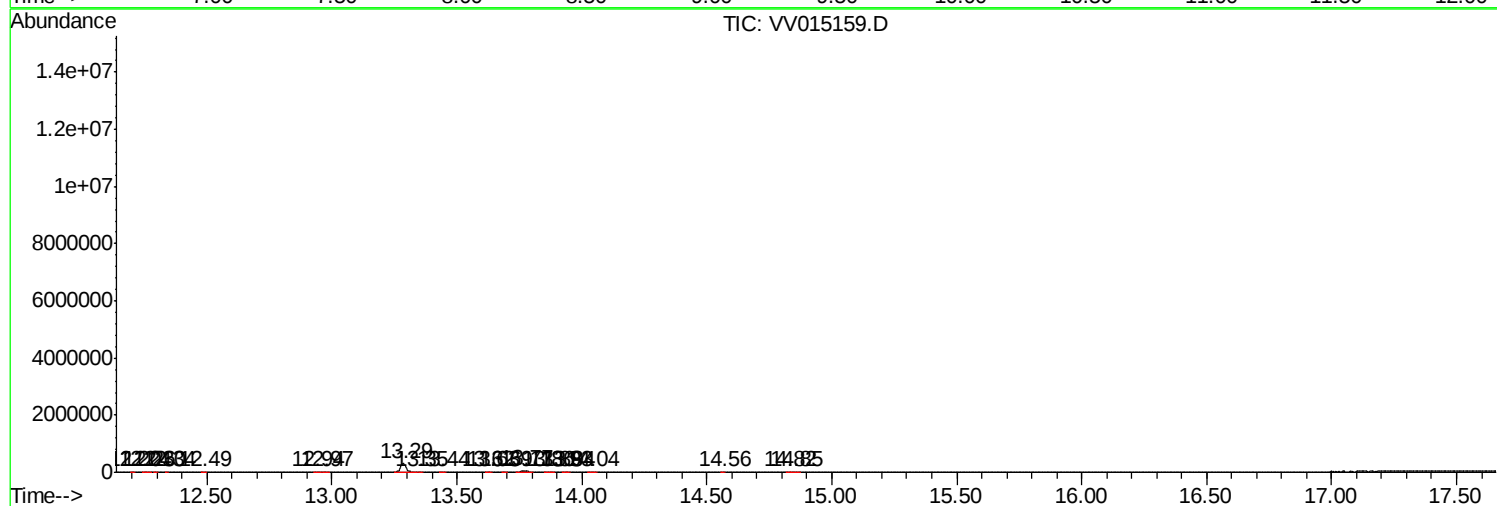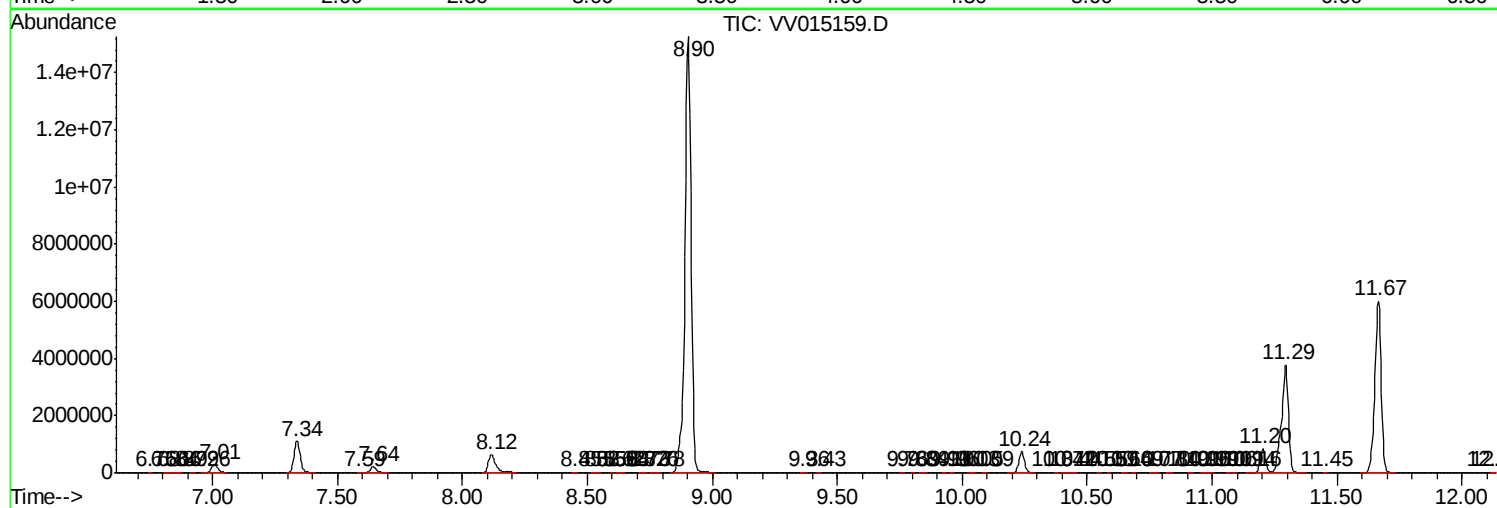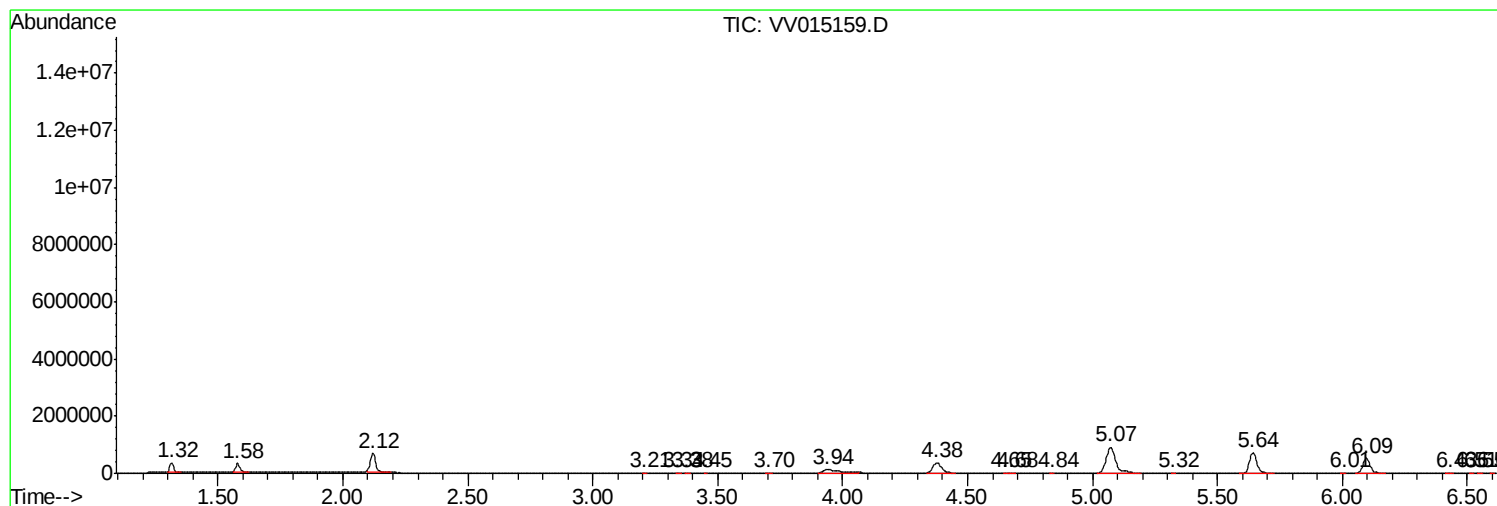

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032520\
Data File : VV015159.D
Acq On : 26 Mar 2020 01:22
Operator : SY/MD
Sample : L1968-14 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DF1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV032520\
Data File : VV015159.D
Acq On : 26 Mar 2020 01:22
Operator : SY/MD
Sample : L1968-14 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DF1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc