

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032520\
 Data File : VV015160.D
 Acq On : 26 Mar 2020 01:46
 Operator : SY/MD
 Sample : L1968-14DL 2000X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DF1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	86	rVB	341791	343954	14.73%	1.815%
2	1.579	146	152	164	rVB	298267	347756	14.89%	1.835%
3	2.119	313	320	334	rVB	617366	867578	37.16%	4.577%
4	3.177	645	649	654	rVB7	2694	2164	0.09%	0.011%
5	3.486	741	745	748	rBV	17659	10118	0.43%	0.053%
6	3.534	758	760	764	rVB5	2110	1184	0.05%	0.006%
7	3.939	874	886	926	rBV	122251	557603	23.88%	2.942%
8	4.376	1008	1022	1046	rVB	353200	869106	37.22%	4.585%
9	4.634	1097	1102	1106	rBV8	2308	3050	0.13%	0.016%
10	4.727	1129	1131	1133	rVB3	1888	738	0.03%	0.004%
11	4.753	1135	1139	1142	rBV5	2253	1849	0.08%	0.010%
12	4.968	1204	1206	1211	rBV5	1180	1141	0.05%	0.006%
13	5.074	1220	1239	1269	rBV2	881864	2199141	94.18%	11.603%
14	5.293	1302	1307	1309	rBV5	2862	2742	0.12%	0.014%
15	5.338	1315	1321	1327	rVB10	2226	2654	0.11%	0.014%
16	5.367	1327	1330	1331	rBV3	1969	1085	0.05%	0.006%
17	5.643	1403	1416	1436	rBV	679546	1353225	57.95%	7.140%
18	6.032	1535	1537	1541	rBV5	1823	1318	0.06%	0.007%
19	6.097	1544	1557	1578	rVV	499981	997708	42.73%	5.264%
20	6.486	1676	1678	1679	rBV2	1361	559	0.02%	0.003%
21	6.756	1758	1762	1765	rBV5	2440	2349	0.10%	0.012%
22	6.884	1796	1802	1809	rBV10	2806	4594	0.20%	0.024%
23	6.926	1814	1815	1817	rBV2	1120	420	0.02%	0.002%
24	7.007	1828	1840	1859	rBV	274302	504311	21.60%	2.661%
25	7.338	1930	1943	1963	rBV	1062464	1847118	79.11%	9.745%
26	7.605	2024	2026	2028	rBV3	1566	698	0.03%	0.004%
27	7.643	2028	2038	2057	rBV	199753	343133	14.70%	1.810%
28	7.810	2088	2090	2091	rBV3	1256	480	0.02%	0.003%
29	7.865	2105	2107	2108	rVB2	783	215	0.01%	0.001%
30	7.881	2108	2112	2113	rBV3	2318	1451	0.06%	0.008%
31	7.958	2133	2136	2142	rBV7	2027	2187	0.09%	0.012%
32	8.055	2164	2166	2171	rVB5	2478	1423	0.06%	0.008%
33	8.116	2174	2185	2216	rVV2	625136	1260073	53.96%	6.648%
34	8.691	2361	2364	2367	rVB4	1761	1385	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032520\
 Data File : VV015160.D
 Acq On : 26 Mar 2020 01:46
 Operator : SY/MD
 Sample : L1968-14DL 2000X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DF1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
 Title : VOC Analysis

35	8.769	2386	2388	2389	rBV2	1423	749	0.03%	0.004%
36	8.875	2409	2421	2425	rBV	1100191	1738066	74.44%	9.170%
37	9.425	2589	2592	2595	rBV4	1131	782	0.03%	0.004%
38	9.460	2601	2603	2606	rVB4	1199	595	0.03%	0.003%
39	9.531	2623	2625	2630	rBV5	1799	1487	0.06%	0.008%
40	9.617	2649	2652	2656	rVB5	2007	1253	0.05%	0.007%
41	9.637	2656	2658	2660	rBV3	1400	798	0.03%	0.004%
42	9.666	2665	2667	2669	rVV3	2415	1187	0.05%	0.006%
43	9.691	2673	2675	2678	rVB4	2295	852	0.04%	0.004%
44	9.785	2701	2704	2705	rBV3	2565	1399	0.06%	0.007%
45	9.846	2721	2723	2725	rBV3	1940	1024	0.04%	0.005%
46	9.884	2733	2735	2738	rBV4	1550	969	0.04%	0.005%
47	9.907	2739	2742	2744	rBV4	2047	1058	0.05%	0.006%
48	9.981	2763	2765	2768	rBV3	1862	1191	0.05%	0.006%
49	10.029	2777	2780	2783	rVB5	2000	877	0.04%	0.005%
50	10.080	2794	2796	2799	rBV4	1306	720	0.03%	0.004%
51	10.138	2809	2814	2816	rBV6	2108	1961	0.08%	0.010%
52	10.238	2834	2845	2865	rVB	710331	1119365	47.94%	5.906%
53	10.341	2872	2877	2879	rBV4	1229	957	0.04%	0.005%
54	10.441	2906	2908	2910	rBV3	1098	661	0.03%	0.003%
55	10.550	2938	2942	2944	rBV5	2721	2374	0.10%	0.013%
56	10.714	2991	2993	2996	rBV4	882	480	0.02%	0.003%
57	10.736	2996	3000	3003	rVV5	2060	2003	0.09%	0.011%
58	10.756	3004	3006	3010	rVV4	2591	1583	0.07%	0.008%
59	10.788	3013	3016	3019	rVB4	2277	1229	0.05%	0.006%
60	10.814	3019	3024	3027	rBV7	1276	1029	0.04%	0.005%
61	10.833	3027	3030	3034	rBV6	1859	1683	0.07%	0.009%
62	11.016	3085	3087	3092	rVB6	1567	992	0.04%	0.005%
63	11.129	3119	3122	3124	rBV4	1936	1238	0.05%	0.007%
64	11.206	3136	3146	3155	rBV2	63858	104473	4.47%	0.551%
65	11.270	3156	3166	3192	rVB2	1041851	2019053	86.47%	10.652%
66	11.473	3222	3229	3230	rBV7	2759	3089	0.13%	0.016%
67	11.540	3246	3250	3251	rBV4	1650	1273	0.05%	0.007%
68	11.650	3271	3284	3310	rBV3	1161681	2334991	100.00%	12.319%
69	12.019	3396	3399	3401	rBV4	2065	1093	0.05%	0.006%
70	12.106	3423	3426	3427	rBV3	1613	995	0.04%	0.005%
71	12.151	3438	3440	3443	rBV4	1346	875	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032520\
 Data File : VV015160.D
 Acq On : 26 Mar 2020 01:46
 Operator : SY/MD
 Sample : L1968-14DL 2000X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DF1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
 Title : VOC Analysis

72	12.177	3446	3448	3450	rBV3	1877	849	0.04%	0.004%
73	12.206	3455	3457	3461	rBV4	1175	790	0.03%	0.004%
74	12.228	3461	3464	3467	rBV5	1949	1686	0.07%	0.009%
75	12.322	3490	3493	3494	rBV3	1626	1076	0.05%	0.006%
76	12.370	3505	3508	3510	rBV3	1790	1033	0.04%	0.005%
77	12.440	3528	3530	3533	rVB4	1023	459	0.02%	0.002%
78	12.527	3554	3557	3558	rBV3	1374	751	0.03%	0.004%
79	12.569	3568	3570	3571	rBV2	1871	749	0.03%	0.004%
80	12.653	3594	3596	3597	rBV2	1465	556	0.02%	0.003%
81	12.875	3662	3665	3667	rBV4	2018	1302	0.06%	0.007%
82	12.997	3698	3703	3706	rBV6	2947	2698	0.12%	0.014%
83	13.035	3712	3715	3717	rBV4	1477	950	0.04%	0.005%
84	13.170	3753	3757	3761	rBV6	2236	2118	0.09%	0.011%
85	13.199	3764	3766	3768	rVV3	1182	534	0.02%	0.003%
86	13.286	3784	3793	3803	rBV4	28240	46246	1.98%	0.244%
87	13.431	3835	3838	3840	rBV4	1596	932	0.04%	0.005%
88	13.736	3931	3933	3937	rBV4	1801	1244	0.05%	0.007%
89	13.993	4011	4013	4015	rBV3	1965	1123	0.05%	0.006%


Sum of corrected areas: 18954010

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032520\
Data File : VV015160.D
Acq On : 26 Mar 2020 01:46
Operator : SY/MD
Sample : L1968-14DL 2000X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DF1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

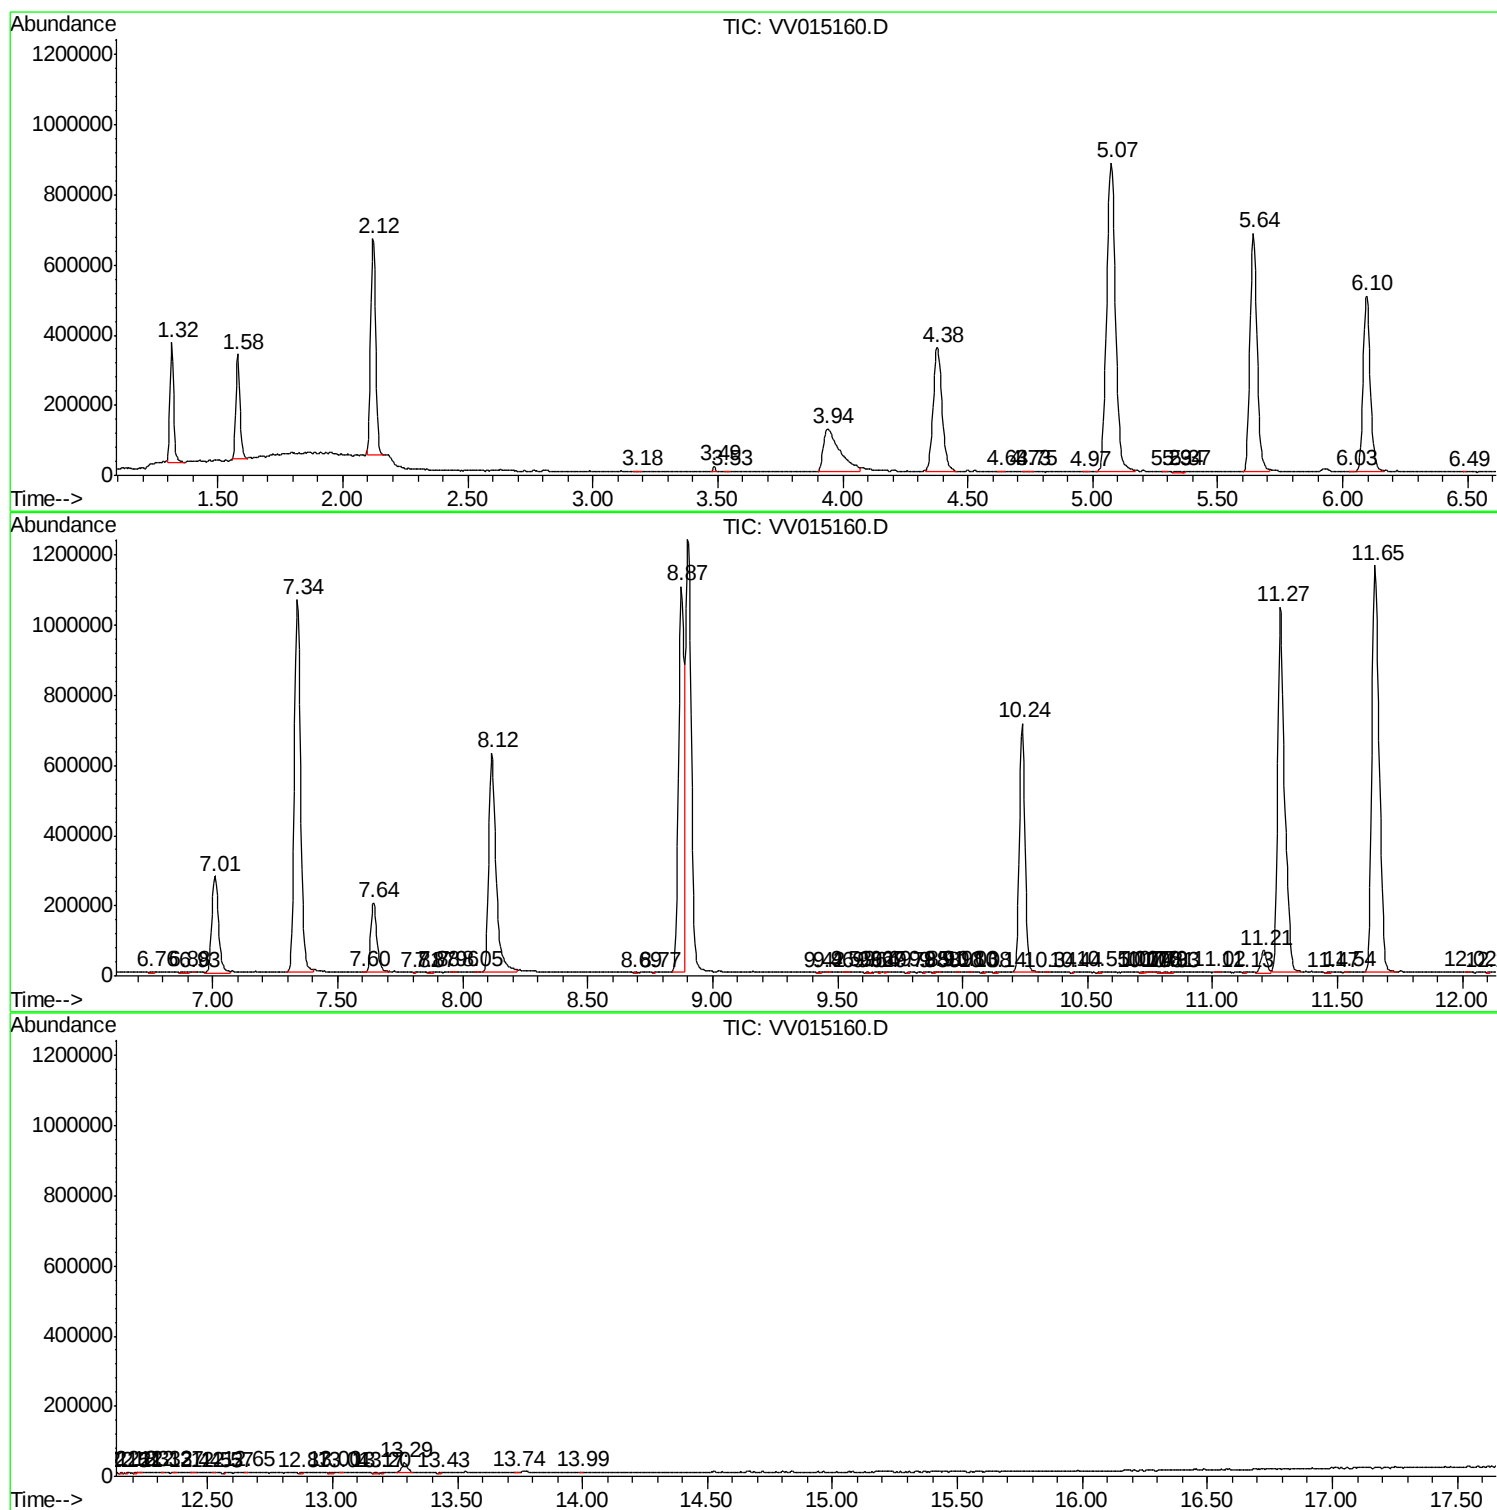

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032520\
Data File : VV015160.D
Acq On : 26 Mar 2020 01:46
Operator : SY/MD
Sample : L1968-14DL 2000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DF1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032520\
Data File : VV015160.D
Acq On : 26 Mar 2020 01:46
Operator : SY/MD
Sample : L1968-14DL 2000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DF1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc