

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032520\
 Data File : VV015161.D
 Acq On : 26 Mar 2020 02:10
 Operator : SY/MD
 Sample : L1968-15 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DL5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	82	rVB	353570	349424	1.66%	0.610%
2	1.579	146	152	165	rVB	295899	344055	1.64%	0.600%
3	2.119	313	320	349	rVB	672576	1066447	5.08%	1.860%
4	3.277	677	680	681	rBV3	2262	1246	0.01%	0.002%
5	3.705	806	813	816	rBV8	3151	3502	0.02%	0.006%
6	3.753	826	828	830	rBV3	2134	925	0.00%	0.002%
7	3.872	862	865	870	rVB6	1658	1493	0.01%	0.003%
8	3.939	874	886	930	rVV2	118904	562593	2.68%	0.981%
9	4.380	1008	1023	1050	rVB	360959	938155	4.47%	1.637%
10	4.811	1153	1157	1160	rBV6	2846	2606	0.01%	0.005%
11	4.930	1192	1194	1196	rBV3	1405	754	0.00%	0.001%
12	5.074	1222	1239	1246	rBV2	883148	2137361	10.17%	3.728%
13	5.643	1403	1416	1442	rBV	721921	1414620	6.73%	2.468%
14	6.026	1532	1535	1541	rBV7	2651	3259	0.02%	0.006%
15	6.097	1543	1557	1581	rVV	499476	1012217	4.82%	1.766%
16	6.344	1630	1634	1639	rBV8	2044	2115	0.01%	0.004%
17	6.412	1654	1655	1658	rVB3	2121	839	0.00%	0.001%
18	6.434	1658	1662	1663	rBV4	1082	802	0.00%	0.001%
19	6.479	1673	1676	1677	rBV3	1849	1011	0.00%	0.002%
20	6.524	1687	1690	1691	rBV3	1338	807	0.00%	0.001%
21	6.569	1702	1704	1708	rBV5	1222	710	0.00%	0.001%
22	6.637	1723	1725	1728	rBV3	2246	1393	0.01%	0.002%
23	6.724	1749	1752	1754	rVB4	1690	908	0.00%	0.002%
24	6.737	1754	1756	1758	rBV3	1655	900	0.00%	0.002%
25	6.765	1762	1765	1767	rBV3	1691	1209	0.01%	0.002%
26	6.804	1774	1777	1779	rBV4	2481	1517	0.01%	0.003%
27	6.881	1798	1801	1804	rBV5	1891	1739	0.01%	0.003%
28	6.910	1808	1810	1811	rBV2	1536	713	0.00%	0.001%
29	7.007	1830	1840	1861	rBV	281363	494839	2.36%	0.863%
30	7.338	1932	1943	1964	rBV	1092530	1859450	8.85%	3.244%
31	7.643	2027	2038	2057	rBV	201183	342965	1.63%	0.598%
32	7.798	2085	2086	2087	rBV	1855	643	0.00%	0.001%
33	7.923	2123	2125	2128	rBV4	1295	701	0.00%	0.001%
34	8.116	2174	2185	2227	rBV2	626094	1265340	6.02%	2.207%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032520\
 Data File : VV015161.D
 Acq On : 26 Mar 2020 02:10
 Operator : SY/MD
 Sample : L1968-15 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DL5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
 Title : VOC Analysis

35	8.386	2266	2269	2273	rBV5	3024	2176	0.01%	0.004%
36	8.421	2278	2280	2283	rVB4	1670	925	0.00%	0.002%
37	8.537	2313	2316	2319	rBV5	2511	1861	0.01%	0.003%
38	8.579	2325	2329	2332	rBV6	2271	1975	0.01%	0.003%
39	8.663	2352	2355	2358	rBV4	2766	2068	0.01%	0.004%
40	8.695	2362	2365	2371	rBV7	1378	1748	0.01%	0.003%
41	8.820	2399	2404	2406	rBV5	2093	1777	0.01%	0.003%
42	8.904	2406	2430	2454	rBV	11935797	21009029	100.00%	36.648%
43	9.363	2569	2573	2574	rBV3	1554	1195	0.01%	0.002%
44	9.408	2585	2587	2592	rBV6	1504	1150	0.01%	0.002%
45	9.431	2592	2594	2599	rBV5	2110	1445	0.01%	0.003%
46	9.524	2620	2623	2626	rVB4	2075	1342	0.01%	0.002%
47	9.543	2626	2629	2633	rBV5	1548	961	0.00%	0.002%
48	9.569	2635	2637	2640	rBV3	2158	1539	0.01%	0.003%
49	9.650	2659	2662	2663	rBV3	1142	658	0.00%	0.001%
50	9.730	2684	2687	2691	rBV5	2271	1889	0.01%	0.003%
51	9.785	2702	2704	2707	rBV4	1250	482	0.00%	0.001%
52	9.852	2720	2725	2729	rBV7	2446	2446	0.01%	0.004%
53	9.945	2752	2754	2758	rBV4	2002	1462	0.01%	0.003%
54	10.238	2829	2845	2863	rBV	731826	1147426	5.46%	2.002%
55	10.482	2919	2921	2927	rVB7	2324	1860	0.01%	0.003%
56	10.511	2928	2930	2936	rVV8	2016	1692	0.01%	0.003%
57	10.550	2939	2942	2945	rBV5	2183	1841	0.01%	0.003%
58	10.566	2945	2947	2952	rVV6	2252	1596	0.01%	0.003%
59	10.688	2982	2985	2987	rVB4	1493	837	0.00%	0.001%
60	10.707	2987	2991	2992	rBV4	2034	1352	0.01%	0.002%
61	10.733	2998	2999	3006	rVB7	1946	1192	0.01%	0.002%
62	10.875	3038	3043	3045	rBV4	3046	3132	0.01%	0.005%
63	10.994	3076	3080	3081	rBV4	841	728	0.00%	0.001%
64	11.051	3094	3098	3100	rBV5	1897	1442	0.01%	0.003%
65	11.161	3129	3132	3133	rBV3	2254	1338	0.01%	0.002%
66	11.203	3133	3145	3156	rVV	568170	858381	4.09%	1.497%
67	11.293	3156	3173	3195	rVB2	5463571	9870699	46.98%	17.218%
68	11.666	3272	3289	3307	rBV2	5760226	10150764	48.32%	17.707%
69	12.232	3462	3465	3466	rBV3	1807	978	0.00%	0.002%
70	12.299	3483	3486	3487	rBV3	1754	1039	0.00%	0.002%
71	12.344	3497	3500	3502	rBV4	1976	1234	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032520\
 Data File : VV015161.D
 Acq On : 26 Mar 2020 02:10
 Operator : SY/MD
 Sample : L1968-15 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DL5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
 Title : VOC Analysis

72	12.376	3508	3510	3512	rBV3	2339	1145	0.01%	0.002%
73	12.421	3516	3524	3534	rVV8	12667	19583	0.09%	0.034%
74	12.514	3550	3553	3555	rBV4	2455	1841	0.01%	0.003%
75	12.582	3571	3574	3575	rBV3	3810	2276	0.01%	0.004%
76	12.672	3594	3602	3610	rBV9	7736	14094	0.07%	0.025%
77	13.032	3712	3714	3716	rBV3	2141	733	0.00%	0.001%
78	13.064	3721	3724	3726	rBV4	2311	1543	0.01%	0.003%
79	13.222	3771	3773	3774	rBV2	1521	602	0.00%	0.001%
80	13.283	3780	3792	3807	rBV	1209429	1848869	8.80%	3.225%
81	13.418	3832	3834	3837	rBV4	2068	1294	0.01%	0.002%
82	13.444	3841	3842	3844	rBV2	1975	750	0.00%	0.001%
83	13.688	3915	3918	3919	rBV3	2597	1598	0.01%	0.003%
84	13.768	3933	3943	3957	rVB	339942	525565	2.50%	0.917%
85	13.881	3975	3978	3981	rBV4	1969	1592	0.01%	0.003%
86	13.894	3981	3982	3987	rVB4	3298	1960	0.01%	0.003%
87	14.174	4065	4069	4071	rBV5	2494	2404	0.01%	0.004%


Sum of corrected areas: 57326766

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032520\
Data File : VV015161.D
Acq On : 26 Mar 2020 02:10
Operator : SY/MD
Sample : L1968-15 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DL5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

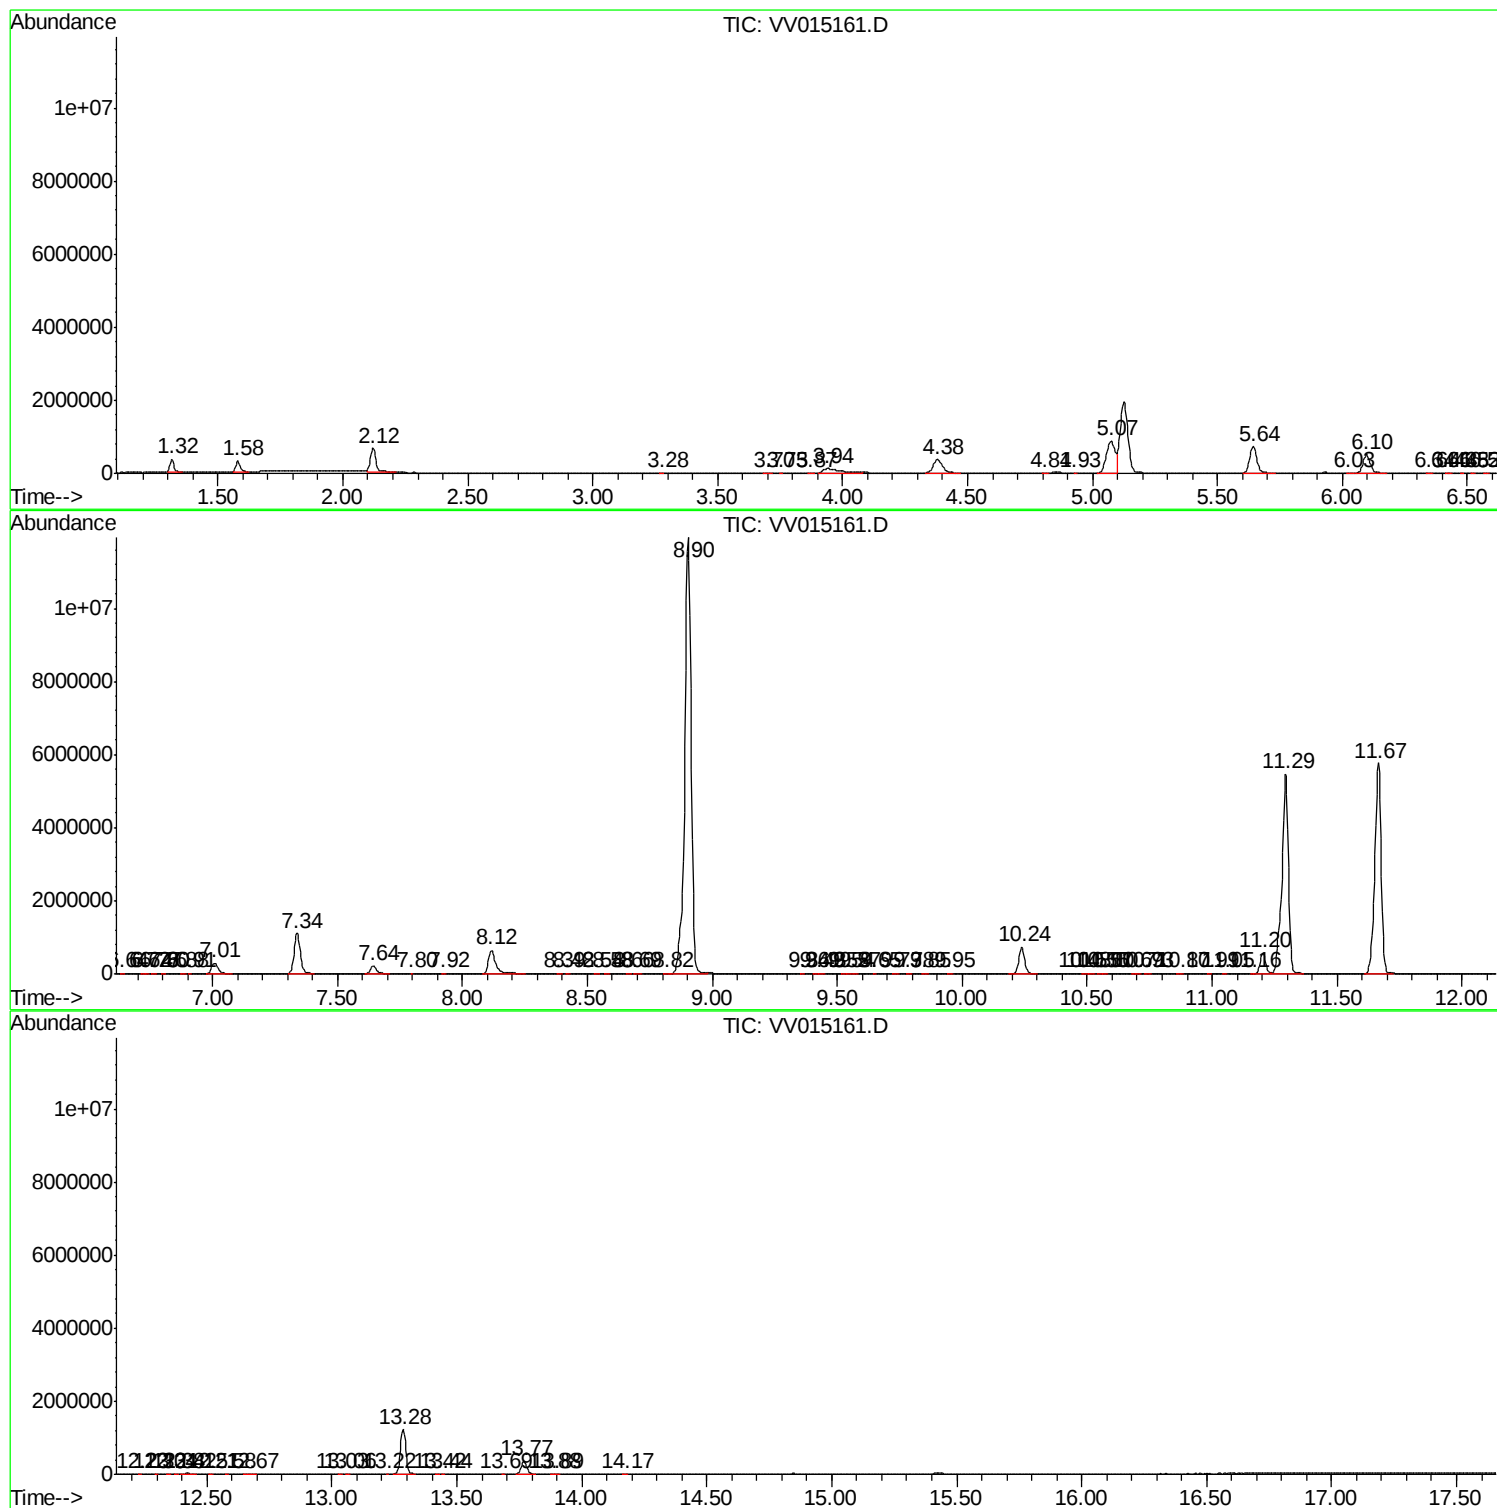

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032520\
Data File : VV015161.D
Acq On : 26 Mar 2020 02:10
Operator : SY/MD
Sample : L1968-15 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DL5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV032520\
Data File : VV015161.D
Acq On : 26 Mar 2020 02:10
Operator : SY/MD
Sample : L1968-15 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DL5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc