


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032520\
 Data File : VV015125.D
 Acq On : 25 Mar 2020 02:57
 Operator : SY/MD
 Sample : BFB71
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB71

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
 Title : VOC Analysis
 Last Update : Tue Mar 31 06:16:11 2020

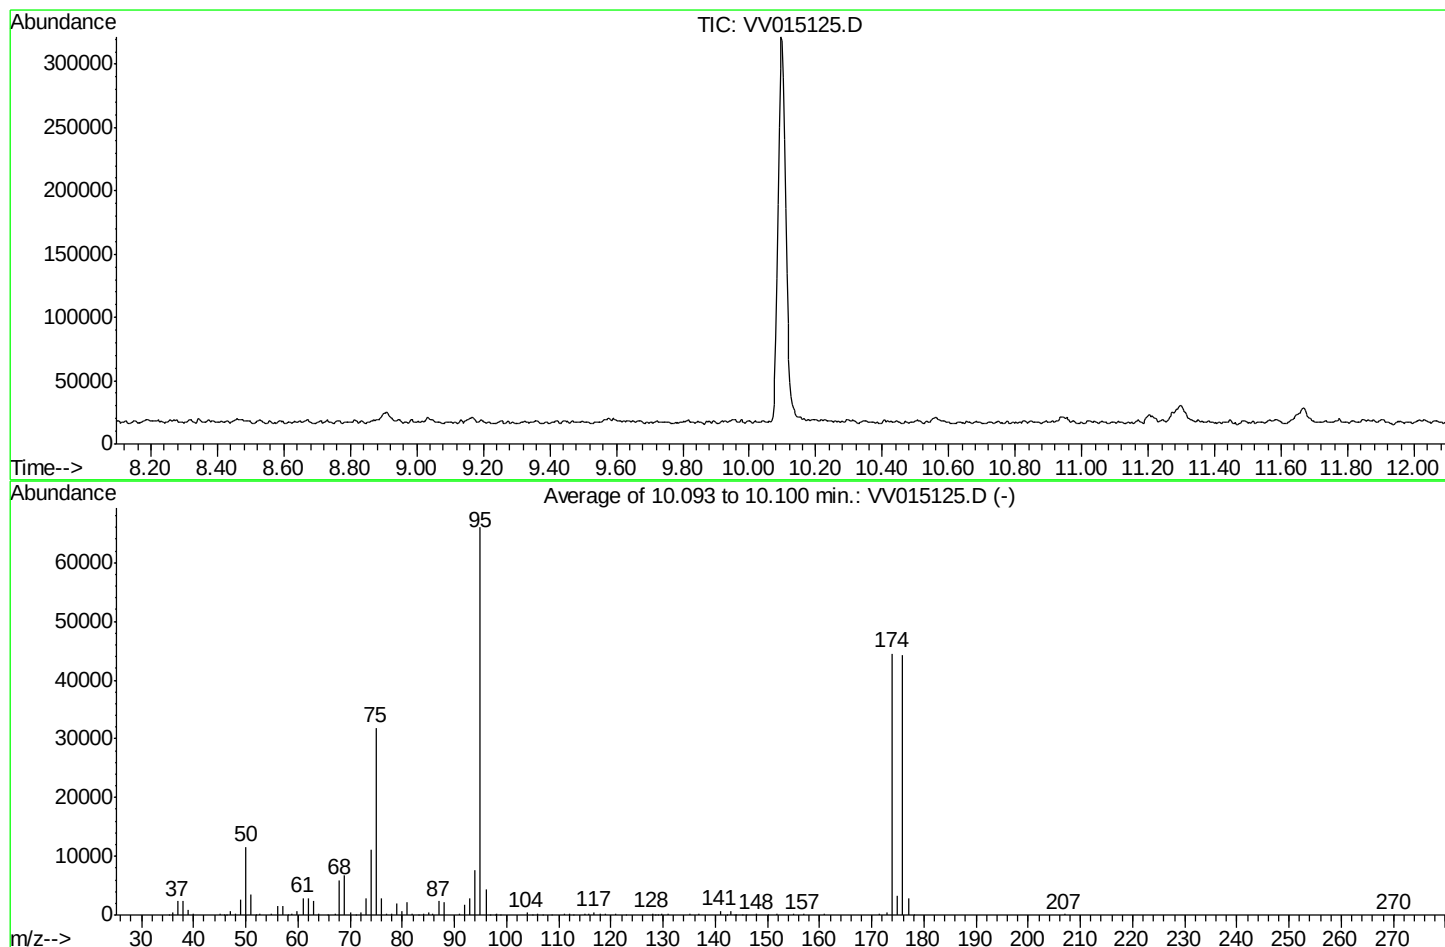

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	11657	PASS
75	95	30	80	48.4	31941	PASS
95	95	100	100	100.0	66024	PASS
96	95	5	9	6.6	4357	PASS
173	174	0.00	2	0.9	417	PASS
174	95	50	120	67.4	44498	PASS
175	174	5	9	7.3	3253	PASS
176	174	95	101	99.7	44357	PASS
177	176	5	9	6.3	2799	PASS

m/z	Abundance
36.10	147.0
36.90	217.0
38.10	246.0
39.00	568.0
40.00	733.0
41.00	921.0
42.10	335.0
43.00	875.0
44.00	1881.0
44.90	380.0
46.10	184.0
48.10	114.0
49.10	117.0
50.00	208.0
51.10	185.0
51.90	132.0
53.00	284.0
53.90	255.0
55.00	639.0
56.30	383.0
57.00	800.0
58.20	168.0
60.00	210.0
64.00	106.0
65.00	156.0
65.80	120.0
67.00	287.0
68.00	320.0
68.90	412.0
70.00	295.0
71.00	389.0
72.80	252.0
73.80	108.0
77.00	223.0
77.60	138.0
79.00	204.0
80.90	289.0
82.00	341.0
83.00	309.0
84.30	213.0
85.30	319.0
87.00	114.0
88.00	103.0
91.00	375.0
92.00	182.0
93.70	101.0
94.90	181.0
96.10	199.0
96.90	279.0
98.90	127.0
102.00	143.0
103.20	108.0
103.70	117.0
104.80	138.0
109.10	141.0
109.80	117.0
113.90	132.0
117.10	103.0
140.20	131.0
149.60	118.0
162.10	106.0
200.40	133.0
241.30	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
35.20	161.0
36.10	649.0
37.00	2558.0
38.00	2604.0
39.00	1406.0
40.00	1069.0
41.00	694.0
42.00	315.0
43.00	920.0
44.00	1835.0
45.00	681.0
46.10	176.0
47.00	746.0
48.00	378.0
49.00	2465.0
50.00	12065.0
51.00	3643.0
51.80	272.0
52.70	127.0
53.10	208.0
54.10	213.0
55.00	925.0
56.00	1595.0
57.00	2484.0
57.90	280.0
58.90	167.0
59.90	817.0
61.00	2923.0
62.00	2834.0
63.00	2280.0
64.10	211.0
65.10	158.0
66.00	103.0
67.10	457.0
68.00	5832.0
69.00	6982.0
70.00	733.0
71.10	390.0
72.20	338.0
73.00	3117.0
74.00	10447.0
75.00	30224.0
76.00	2953.0
77.00	523.0
77.90	310.0
78.90	2060.0
79.90	502.0
80.90	2416.0
81.90	583.0
83.00	429.0
84.00	323.0
85.00	377.0
85.90	237.0
87.00	2173.0
88.00	2000.0
90.90	553.0
92.00	1906.0
93.00	2958.0
94.00	6893.0
95.00	63280.0
96.00	4518.0
97.00	445.0
98.20	227.0
99.00	175.0
103.90	426.0
105.00	191.0
106.00	328.0
106.80	135.0
109.10	200.0
109.90	136.0
111.00	161.0
112.00	170.0
112.90	124.0
115.00	235.0
115.90	297.0
116.80	397.0
117.90	204.0
118.80	234.0
121.00	112.0
122.90	133.0
128.00	280.0
128.60	132.0
129.80	241.0
130.90	165.0
135.20	136.0
137.00	164.0
140.90	604.0
142.10	154.0
142.90	664.0
143.80	124.0
145.10	107.0
147.90	209.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

151.80	142.0
154.90	179.0
156.90	206.0
160.90	111.0
171.50	163.0
174.00	40592.0
174.90	2982.0
175.90	40848.0
177.00	2531.0
178.00	115.0
207.00	199.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
36.10	582.0
37.00	2713.0
38.00	2706.0
39.00	1483.0
40.00	950.0
41.00	729.0
42.00	244.0
43.00	857.0
44.00	1656.0
45.10	733.0
46.10	121.0
47.00	799.0
48.00	403.0
49.00	2794.0
50.00	12347.0
51.00	3748.0
51.90	230.0
52.70	163.0
53.20	216.0
54.10	247.0
55.00	976.0
56.10	1610.0
57.00	2450.0
58.00	266.0
58.90	172.0
59.90	782.0
61.00	2908.0
62.00	3011.0
63.00	2561.0
63.90	212.0
65.10	145.0
65.80	117.0
67.20	376.0
68.00	6315.0
69.00	7487.0
70.10	742.0
71.10	437.0
72.10	390.0
73.00	3059.0
74.00	11694.0
75.00	33056.0
76.00	3017.0
77.00	518.0
77.90	306.0
78.90	2205.0
79.90	614.0
80.90	2430.0
81.90	688.0
83.00	405.0
84.00	288.0
85.00	397.0
85.90	249.0
87.00	2452.0
88.00	2330.0
90.90	539.0
92.00	2052.0
93.00	2961.0
94.00	7693.0
95.00	68584.0
96.00	4595.0
97.00	372.0
98.10	227.0
98.90	159.0
103.90	507.0
104.90	249.0
105.90	328.0
106.80	109.0
109.20	140.0
111.00	217.0
112.00	172.0
112.90	117.0
114.90	169.0
115.80	270.0
116.80	409.0
117.90	226.0
118.90	345.0
121.00	126.0
127.90	308.0
129.10	123.0
129.80	254.0
130.90	194.0
135.20	133.0
136.90	219.0
140.90	715.0
142.20	120.0
142.90	679.0
144.00	117.0
145.80	108.0
147.90	224.0
151.80	149.0
154.90	225.0
156.90	212.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

160.90	139.0
171.50	157.0
173.00	622.0
174.00	45864.0
174.90	3343.0
176.00	45720.0
177.00	2889.0
207.00	196.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
36.00	579.0
37.00	2536.0
38.00	2542.0
39.00	1573.0
39.90	852.0
41.00	754.0
42.00	335.0
43.00	806.0
44.00	1657.0
45.10	713.0
45.70	145.0
46.30	133.0
47.00	716.0
48.00	382.0
49.00	2870.0
50.00	11184.0
51.00	3593.0
51.80	201.0
52.70	169.0
53.30	176.0
54.10	286.0
55.00	848.0
56.10	1443.0
57.00	2386.0
58.10	256.0
58.90	145.0
59.90	725.0
61.00	2788.0
62.00	2999.0
63.00	2475.0
63.90	254.0
65.20	135.0
65.70	150.0
66.90	410.0
68.00	6576.0
69.00	7022.0
70.10	788.0
71.10	424.0
72.10	396.0
73.00	2807.0
74.00	11749.0
75.00	32544.0
76.10	2735.0
77.00	506.0
78.90	2218.0
79.90	672.0
80.90	2301.0
81.90	728.0
83.00	305.0
84.00	234.0
85.10	424.0
85.90	287.0
87.00	2637.0
88.00	2308.0
90.90	435.0
92.00	1910.0
93.00	2849.0
94.00	8117.0
95.00	66752.0
96.00	4556.0
97.00	348.0
97.90	216.0
98.90	140.0
103.20	113.0
103.90	547.0
104.90	276.0
105.80	348.0
108.70	103.0
111.10	280.0
112.00	153.0
113.80	120.0
114.80	119.0
115.80	251.0
116.80	514.0
118.00	247.0
118.90	418.0
120.90	124.0
127.80	359.0
129.00	130.0
129.80	269.0
130.90	172.0
135.20	121.0
137.00	200.0
140.90	743.0
143.00	670.0
144.00	157.0
145.80	108.0
147.90	211.0
150.10	134.0
151.80	117.0
154.90	226.0
156.90	215.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

160.90	142.0
171.50	153.0
173.00	629.0
174.00	47040.0
174.90	3436.0
176.00	46504.0
177.00	2978.0
207.00	135.0
270.20	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71