


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032520\
Data File : VV015132.D
Acq On : 25 Mar 2020 08:52
Operator : SY/MD
Sample : BFB72
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB72

Integration File: LSCINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032520WMA.M
Title : VOC Analysis
Last Update : Tue Mar 31 06:16:11 2020

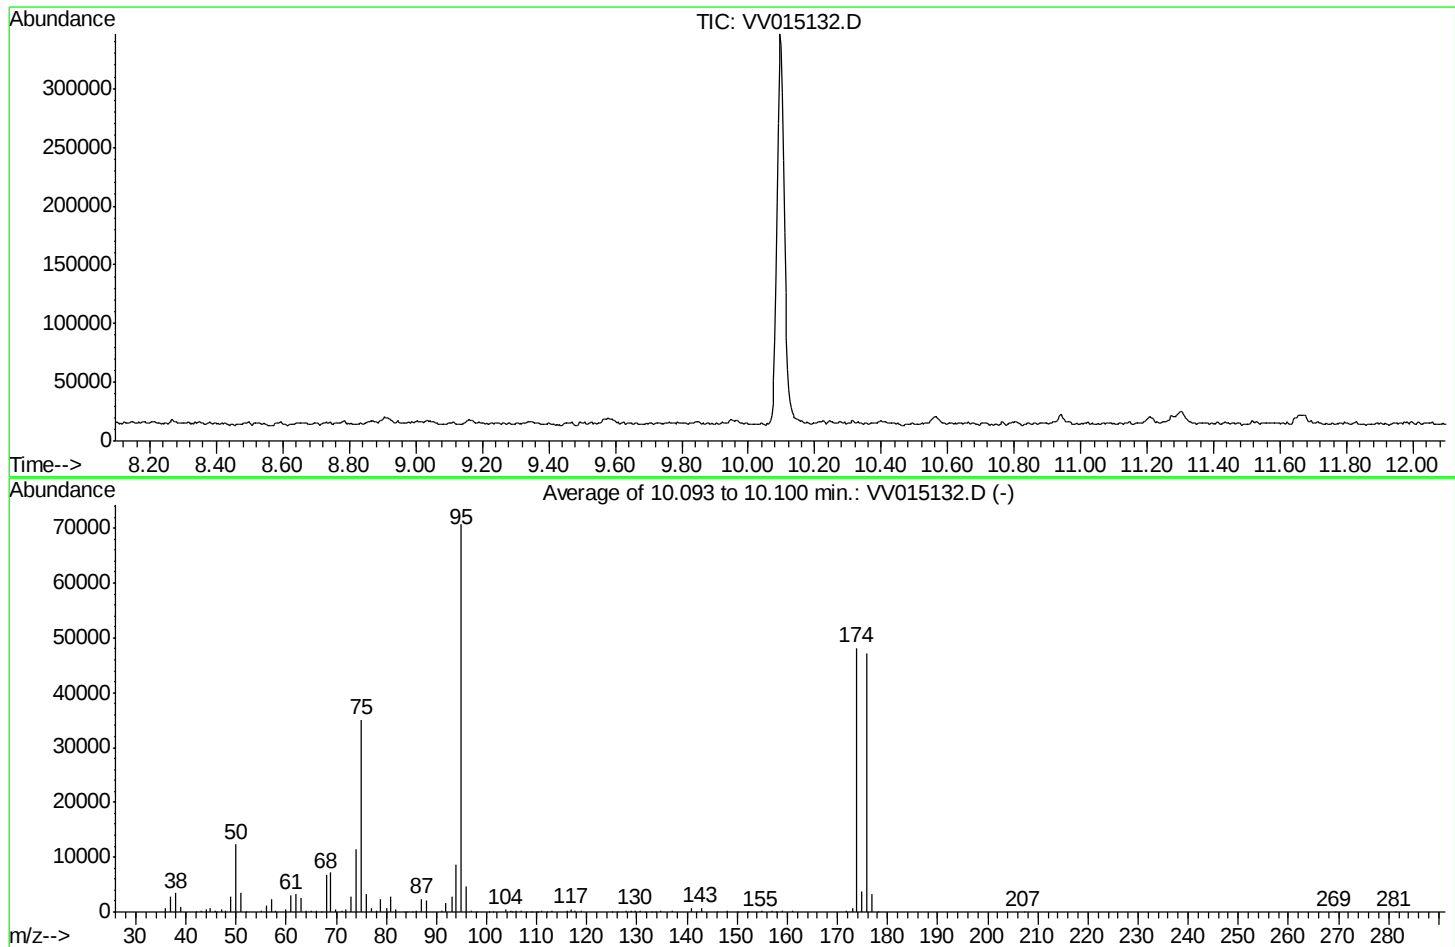

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	12367	PASS
75	95	30	80	49.6	35079	PASS
95	95	100	100	100.0	70704	PASS
96	95	5	9	6.5	4611	PASS
173	174	0.00	2	1.5	717	PASS
174	95	50	120	68.0	48109	PASS
175	174	5	9	8.0	3848	PASS
176	174	95	101	97.9	47077	PASS
177	176	5	9	6.9	3249	PASS

m/z	Abundance
35.70	120.0
36.90	202.0
38.00	155.0
39.10	420.0
39.90	962.0
41.00	980.0
41.90	434.0
43.00	812.0
44.00	1330.0
45.10	237.0
47.90	130.0
50.90	148.0
52.00	208.0
53.00	209.0
54.10	258.0
55.00	479.0
56.00	308.0
57.10	565.0
57.90	118.0
59.90	217.0
60.80	134.0
63.90	153.0
65.10	105.0
67.20	293.0
68.00	160.0
68.90	382.0
69.90	221.0
71.00	267.0
72.90	175.0
74.30	147.0
75.00	105.0
77.20	194.0
78.90	118.0
80.00	134.0
81.00	175.0
82.10	185.0
83.00	361.0
84.00	156.0
85.20	204.0
90.90	221.0
93.10	160.0
93.80	128.0
95.80	165.0
96.10	190.0
97.00	146.0
98.00	161.0
98.90	102.0
103.00	149.0
112.10	130.0
113.60	107.0
114.90	157.0
117.30	102.0
122.90	124.0
127.90	101.0
207.30	151.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
36.00	585.0
37.10	2997.0
38.00	3610.0
39.00	1524.0
39.90	931.0
41.00	577.0
42.00	465.0
43.00	988.0
44.00	1799.0
45.00	926.0
45.90	222.0
47.00	669.0
47.90	436.0
49.00	2708.0
50.00	12140.0
51.00	3379.0
52.00	292.0
52.90	218.0
53.90	145.0
55.10	704.0
56.00	1521.0
57.00	2774.0
58.00	266.0
60.00	704.0
61.00	3095.0
62.00	3462.0
63.00	2467.0
64.00	379.0
65.00	189.0
66.20	126.0
67.00	309.0
68.00	6612.0
69.00	6960.0
70.00	656.0
71.10	410.0
72.00	446.0
73.10	3095.0
74.00	11623.0
75.00	34072.0
76.00	3225.0
77.00	518.0
78.00	262.0
78.90	2443.0
80.00	709.0
80.90	2975.0
81.90	547.0
83.00	263.0
83.70	139.0
84.20	162.0
85.10	226.0
86.10	164.0
87.00	2281.0
88.00	1922.0
91.00	332.0
92.00	1579.0
93.00	2648.0
94.00	8547.0
95.00	68824.0
96.00	4622.0
97.00	414.0
98.00	164.0
101.20	110.0
103.90	430.0
104.80	118.0
105.80	336.0
106.90	172.0
107.80	102.0
109.90	111.0
110.90	170.0
112.00	172.0
113.00	119.0
114.80	181.0
116.00	288.0
116.80	530.0
117.80	223.0
118.90	339.0
126.00	110.0
127.90	273.0
128.90	161.0
129.80	247.0
130.80	199.0
131.70	116.0
132.90	152.0
134.80	169.0
137.00	183.0
140.80	563.0
142.80	784.0
146.00	106.0
147.90	109.0
150.10	107.0
152.10	129.0
155.00	221.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

157.00	207.0
157.60	110.0
158.90	169.0
161.00	224.0
171.80	142.0
173.00	728.0
173.90	45520.0
174.90	3827.0
175.90	43608.0
176.90	3374.0
207.10	257.0
281.30	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
35.90	689.0
37.10	3144.0
38.00	3729.0
39.00	1396.0
39.90	948.0
41.00	610.0
42.00	491.0
43.10	956.0
44.00	1799.0
44.90	1015.0
45.90	232.0
47.10	570.0
47.90	394.0
49.00	2837.0
50.00	12722.0
51.00	3853.0
52.00	320.0
53.00	177.0
53.90	140.0
55.10	701.0
56.00	1481.0
57.00	3103.0
58.00	272.0
60.00	721.0
61.00	3411.0
62.00	3346.0
63.00	2571.0
64.10	303.0
65.00	262.0
66.10	171.0
67.10	309.0
68.00	7213.0
69.00	8016.0
70.00	573.0
71.10	426.0
72.00	475.0
73.10	3072.0
74.00	11766.0
75.00	36520.0
76.00	3386.0
76.90	619.0
78.00	248.0
78.90	2621.0
80.00	761.0
80.90	3208.0
81.90	629.0
83.00	317.0
84.20	186.0
85.00	282.0
86.00	237.0
87.00	2533.0
88.00	2234.0
91.00	406.0
91.90	1660.0
93.00	3054.0
94.00	9084.0
95.00	73224.0
96.00	5230.0
97.10	407.0
97.90	200.0
99.10	137.0
103.90	433.0
104.80	126.0
105.10	119.0
105.80	324.0
106.80	142.0
109.90	126.0
110.90	142.0
112.00	149.0
113.10	133.0
114.70	146.0
116.00	325.0
116.90	516.0
117.80	262.0
118.80	354.0
128.00	284.0
128.90	191.0
129.70	296.0
130.70	186.0
131.70	120.0
132.90	107.0
133.80	108.0
134.90	154.0
136.90	171.0
140.90	672.0
142.80	879.0
146.00	116.0
148.00	151.0
152.10	128.0
154.90	225.0
156.90	179.0
158.90	162.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

161.00	224.0
171.80	185.0
173.00	752.0
173.90	50032.0
174.90	3988.0
175.90	48984.0
176.90	3348.0
207.10	203.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
35.90	748.0
37.00	3090.0
38.00	3320.0
39.00	1264.0
39.90	942.0
40.90	723.0
42.00	458.0
43.10	890.0
44.00	1874.0
45.00	979.0
46.10	188.0
47.20	525.0
47.90	399.0
49.00	2816.0
50.00	12241.0
51.00	3922.0
52.00	301.0
53.00	184.0
53.90	126.0
55.00	727.0
56.00	1336.0
57.00	3081.0
57.90	268.0
60.00	690.0
61.00	3243.0
62.00	3310.0
63.00	2503.0
64.00	286.0
65.00	254.0
66.10	171.0
67.10	334.0
68.00	7240.0
69.00	7941.0
70.00	564.0
71.10	367.0
72.00	515.0
73.00	2961.0
74.00	11037.0
75.00	34960.0
76.00	3180.0
77.00	640.0
78.00	264.0
78.90	2613.0
80.00	756.0
80.90	2920.0
81.90	647.0
83.00	318.0
84.10	159.0
85.00	379.0
86.10	245.0
87.00	2459.0
88.00	2312.0
91.00	404.0
91.90	1773.0
93.00	3157.0
94.00	8544.0
95.00	70064.0
96.00	5046.0
97.10	412.0
97.90	221.0
99.10	154.0
100.60	113.0
103.80	362.0
104.80	145.0
105.00	133.0
105.80	276.0
106.90	126.0
108.90	112.0
109.90	108.0
110.10	111.0
110.90	124.0
111.90	100.0
113.10	140.0
114.70	135.0
116.00	369.0
117.00	512.0
117.70	277.0
118.80	350.0
122.90	115.0
125.00	129.0
128.00	321.0
128.90	177.0
129.80	341.0
130.70	164.0
131.70	108.0
133.80	126.0
134.90	132.0
136.90	148.0
140.90	728.0
141.90	108.0
142.80	813.0
146.10	119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

148.00	170.0
154.80	195.0
156.80	161.0
158.90	174.0
161.00	184.0
171.80	179.0
173.00	673.0
173.90	48776.0
174.90	3729.0
175.90	48640.0
176.90	3026.0
178.10	109.0
207.10	119.0
269.30	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72