

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032522\
 Data File : VW025187.D
 Acq On : 25 Mar 2022 18:50
 Operator : SY/MD
 Sample : N2097-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD9

Manual Integrations
 APPROVED

Reviewed By : John Carlone 03/26/2022
 Supervised By : Mahesh Dadoda 03/31/2022

Quant Time: Mar 25 23:24:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 25 23:19:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	126905	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	123725	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	55554	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	42776	4.270	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	85.400%	
7) Chloroethane-d5	1.568	69	41457	5.651	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	113.000%	
11) 1,1-Dichloroethene-d2	2.108	63	57947	3.579	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	71.600%	
20) 2-Butanone-d5	3.905	46	117609	97.131	ug/L	0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	194.260%#	
24) Chloroform-d	4.352	84	101666	6.118	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	122.400%	
26) 1,2-Dichloroethane-d4	5.037	65	46363	6.674	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	133.400%#	
32) Benzene-d6	5.053	84	197700	5.508	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	110.200%	
36) 1,2-Dichloropropane-d6	6.072	67	62575	6.063	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	121.200%	
41) Toluene-d8	7.317	98	161831	4.947	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	99.000%	
43) trans-1,3-Dichloroprop...	7.628	79	17093	4.751	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	95.000%	
46) 2-Hexanone-d5	8.088	63	91859	74.851	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	149.700%#	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	46054	7.585	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	151.800%#	
66) 1,2-Dichlorobenzene-d4	11.622	152	61876	6.579	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	131.600%#	
Target Compounds						
9) Trichlorofluoromethane	1.757	101	977	0.064	ug/L	90
17) Methyl tert-butyl Ether	2.777	73	1289	0.073	ug/L #	75
25) Chloroform	4.375	83	3270m	0.190	ug/L	
47) Tetrachloroethene	7.979	164	2014	0.267	ug/L	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032522\
Data File : VV025187.D
Acq On : 25 Mar 2022 18:50
Operator : SY/MD
Sample : N2097-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
C0AD9

Manual Integrations
APPROVED

Reviewed By : John Carlone 03/26/2022
Supervised By : Mahesh Dadoda 03/31/2022


Quant Time: Mar 25 23:24:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 25 23:19:44 2022
Response via : Initial Calibration

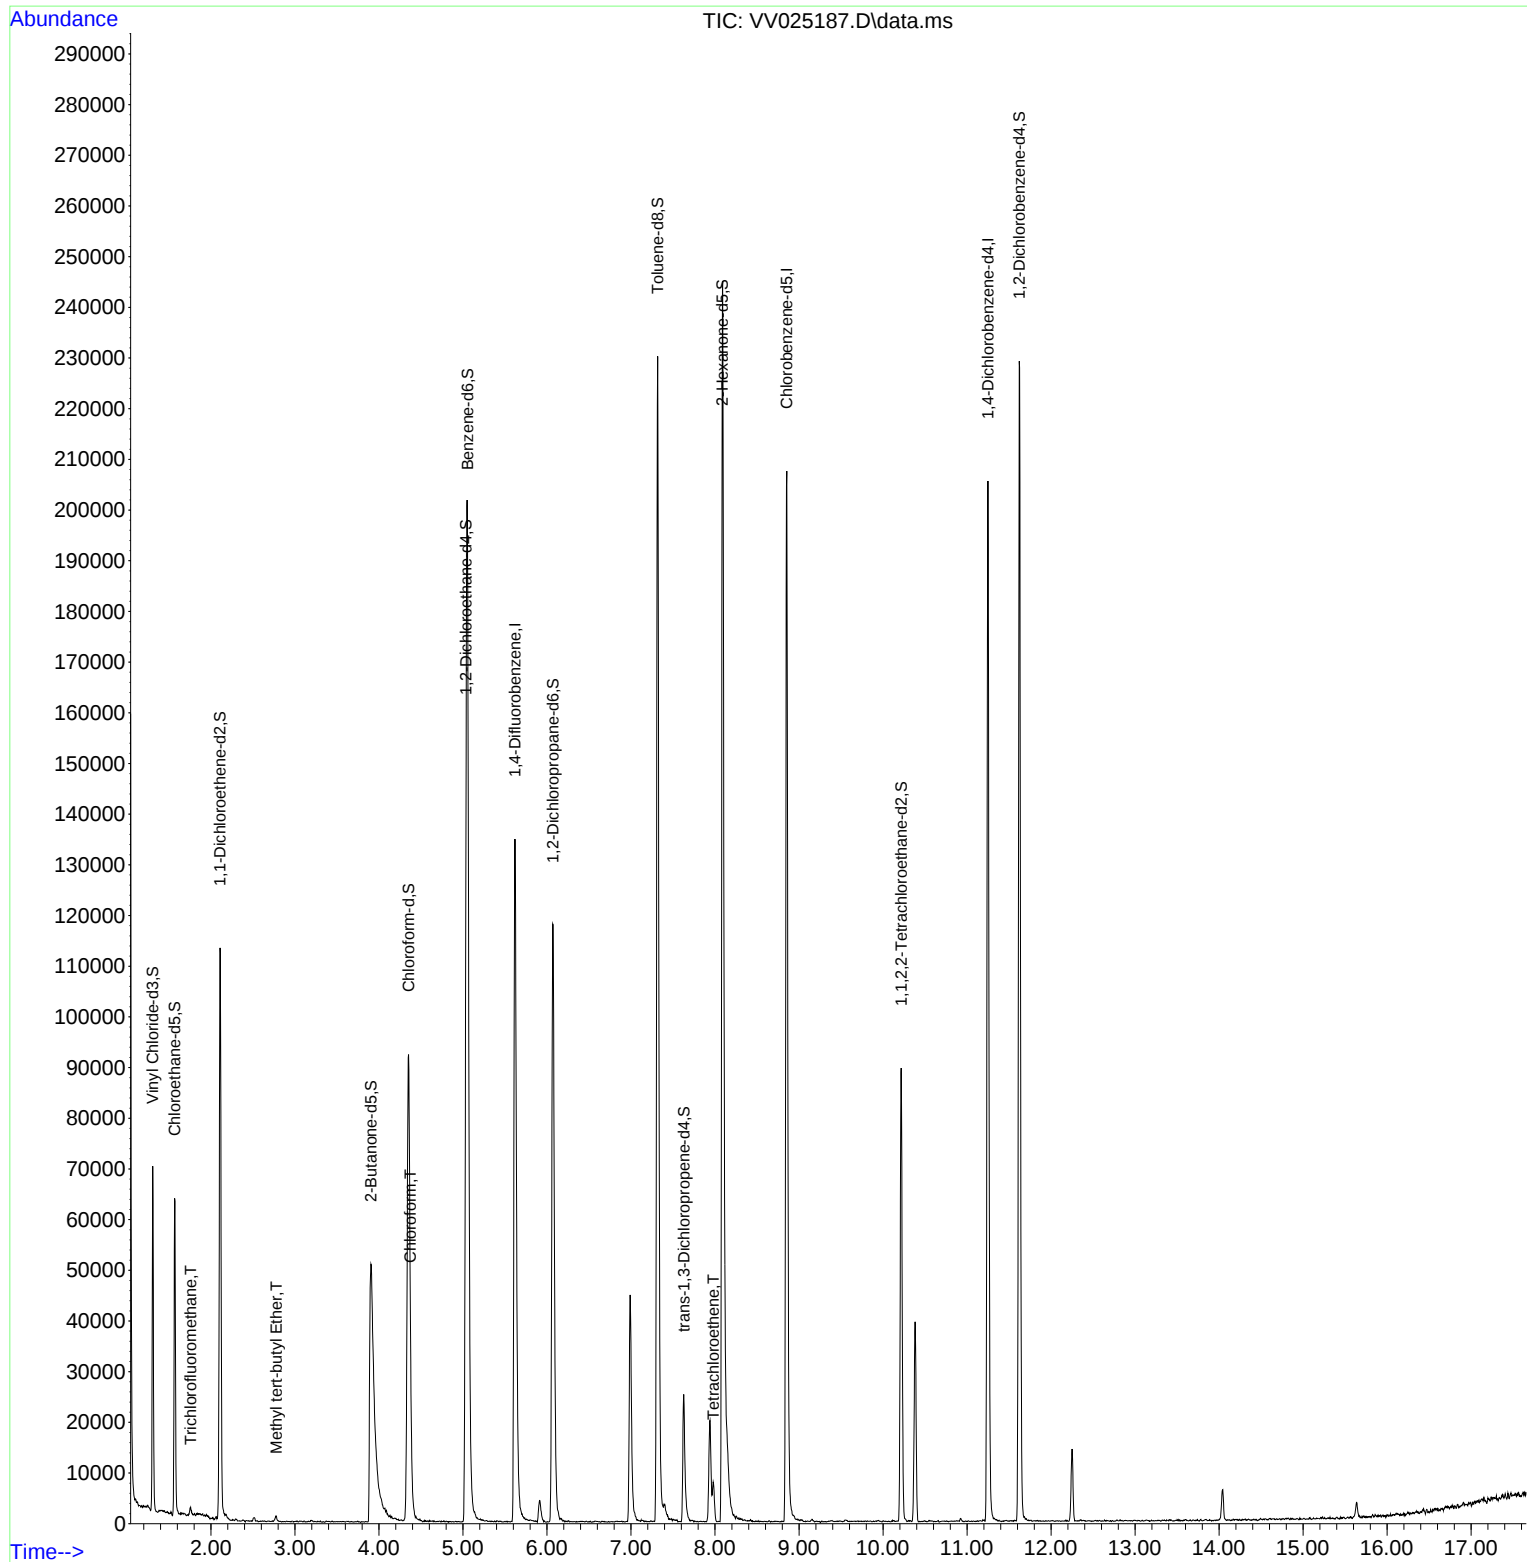

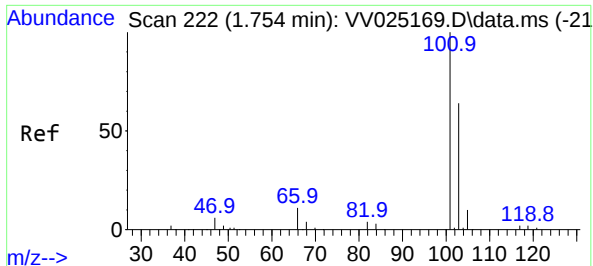

#9
Trichlorofluoromethane
Concen: 0.064 ug/L
RT: 1.757 min Scan# 21
Delta R.T. 0.003 min
Lab File: VV025187.D
Acq: 25 Mar 2022 18:50




Instrument :
MSVOA_V
ClientSampleId :
C0AD9

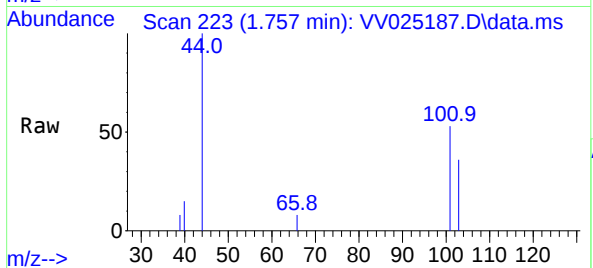


Tgt Ion:101 Resp: 97
Ion Ratio Lower Upper
101 100
103 72.1 51.5 77.3

Manual Integrations
APPROVED



Reviewed By :John Carlone 03/26/2022
Supervised By :Mahesh Dadoda 03/31/2022

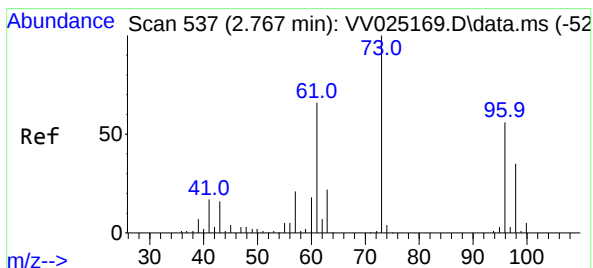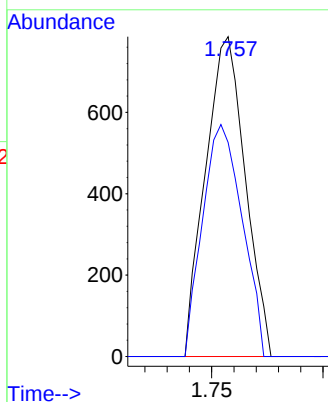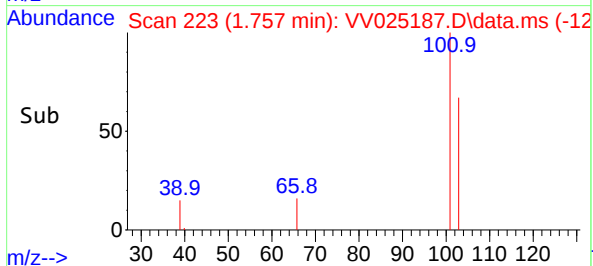


#17
Methyl tert-butyl Ether
Concen: 0.073 ug/L
RT: 2.777 min Scan# 540
Delta R.T. 0.010 min
Lab File: VV025187.D
Acq: 25 Mar 2022 18:50

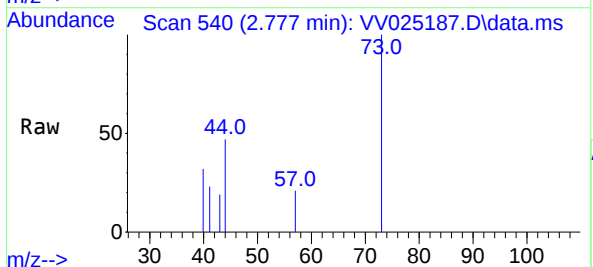

Tgt Ion: 73 Resp: 1289
Ion Ratio Lower Upper
73 100
43 5.6 13.2 19.8#
57 9.5 16.7 25.1#

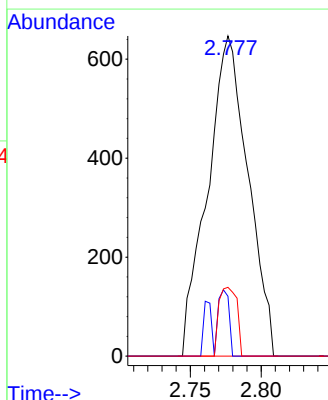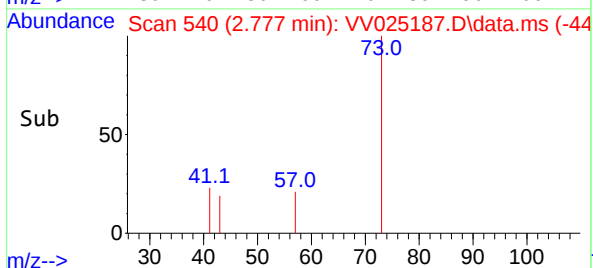

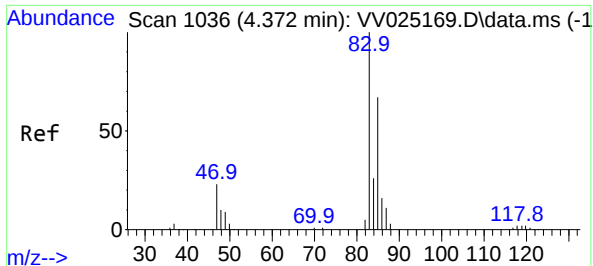

#25

Chloroform

Concen: 0.190 ug/L m

RT: 4.375 min Scan# 1036

Delta R.T. 0.003 min

Lab File: VV025187.D

Acq: 25 Mar 2022 18:50

Instrument :

MSVOA_V

ClientSampleId :

C0AD9

Tgt Ion: 83 Resp: 3270

Ion Ratio Lower Upper

83 100





85 79.4 44.5 82.7

Manual Integrations

APPROVED

Reviewed By :John Carlone 03/26/2022

Supervised By :Mahesh Dadoda 03/31/2022

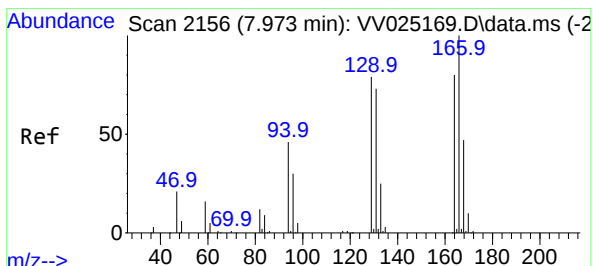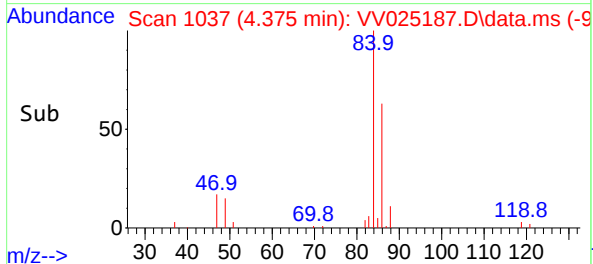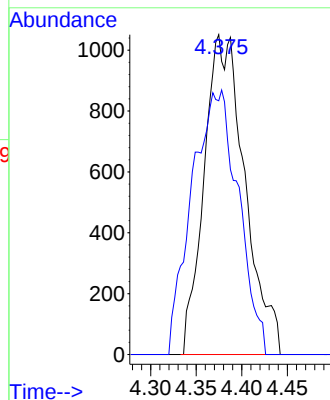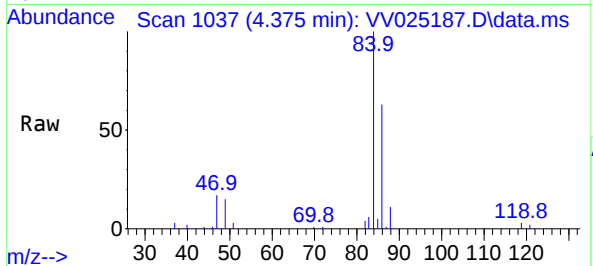

#47

Tetrachloroethene

Concen: 0.267 ug/L

RT: 7.979 min Scan# 2158

Delta R.T. 0.006 min

Lab File: VV025187.D

Acq: 25 Mar 2022 18:50

Tgt Ion:164 Resp: 2014

Ion Ratio Lower Upper

164 100

129 80.7 70.3 130.7

131 94.6 69.4 129.0

166 96.5 90.3 167.7

