

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032522\
 Data File : VV025187.D
 Acq On : 25 Mar 2022 18:50
 Operator : SY/MD
 Sample : N2097-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025187.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	68164	67681	13.44%	1.650%
2	1.568	156	164	178	rBV	62589	72773	14.45%	1.775%
3	2.108	322	332	348	rBV	112537	162860	32.34%	3.972%
4	3.905	880	891	939	rBV2	50842	204013	40.51%	4.975%
5	4.352	1009	1030	1055	rBV	92017	230959	45.86%	5.632%
6	5.050	1231	1247	1273	rBV2	201564	503627	100.00%	12.282%
7	5.619	1413	1424	1449	rBV	134638	276855	54.97%	6.751%
8	5.912	1507	1515	1530	rBV6	4240	8845	1.76%	0.216%
9	6.069	1549	1564	1590	rBV	118015	242964	48.24%	5.925%
10	6.989	1841	1850	1875	rBV	44684	84363	16.75%	2.057%
11	7.317	1941	1952	1974	rBV	229884	403460	80.11%	9.839%
12	7.628	2039	2049	2071	rBV	25123	45708	9.08%	1.115%
13	7.940	2132	2146	2153	rBV	20020	35907	7.13%	0.876%
14	7.979	2154	2158	2170	rVB4	7851	11972	2.38%	0.292%
15	8.091	2183	2193	2232	rBV	244689	485144	96.33%	11.831%
16	8.854	2419	2430	2454	rBV	207264	343566	68.22%	8.378%
17	10.217	2842	2854	2875	rVB	89485	142482	28.29%	3.475%
18	10.381	2893	2905	2918	rVB	39467	63951	12.70%	1.560%
19	11.249	3164	3175	3196	rBV	205263	320214	63.58%	7.809%
20	11.622	3280	3291	3309	rBV	228855	360802	71.64%	8.799%
21	12.249	3475	3486	3496	rBV2	14243	22007	4.37%	0.537%
22	14.043	4029	4044	4059	rVB	6111	10501	2.09%	0.256%


Sum of corrected areas: 4100654

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032522\
Data File : VV025187.D
Acq On : 25 Mar 2022 18:50
Operator : SY/MD
Sample : N2097-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

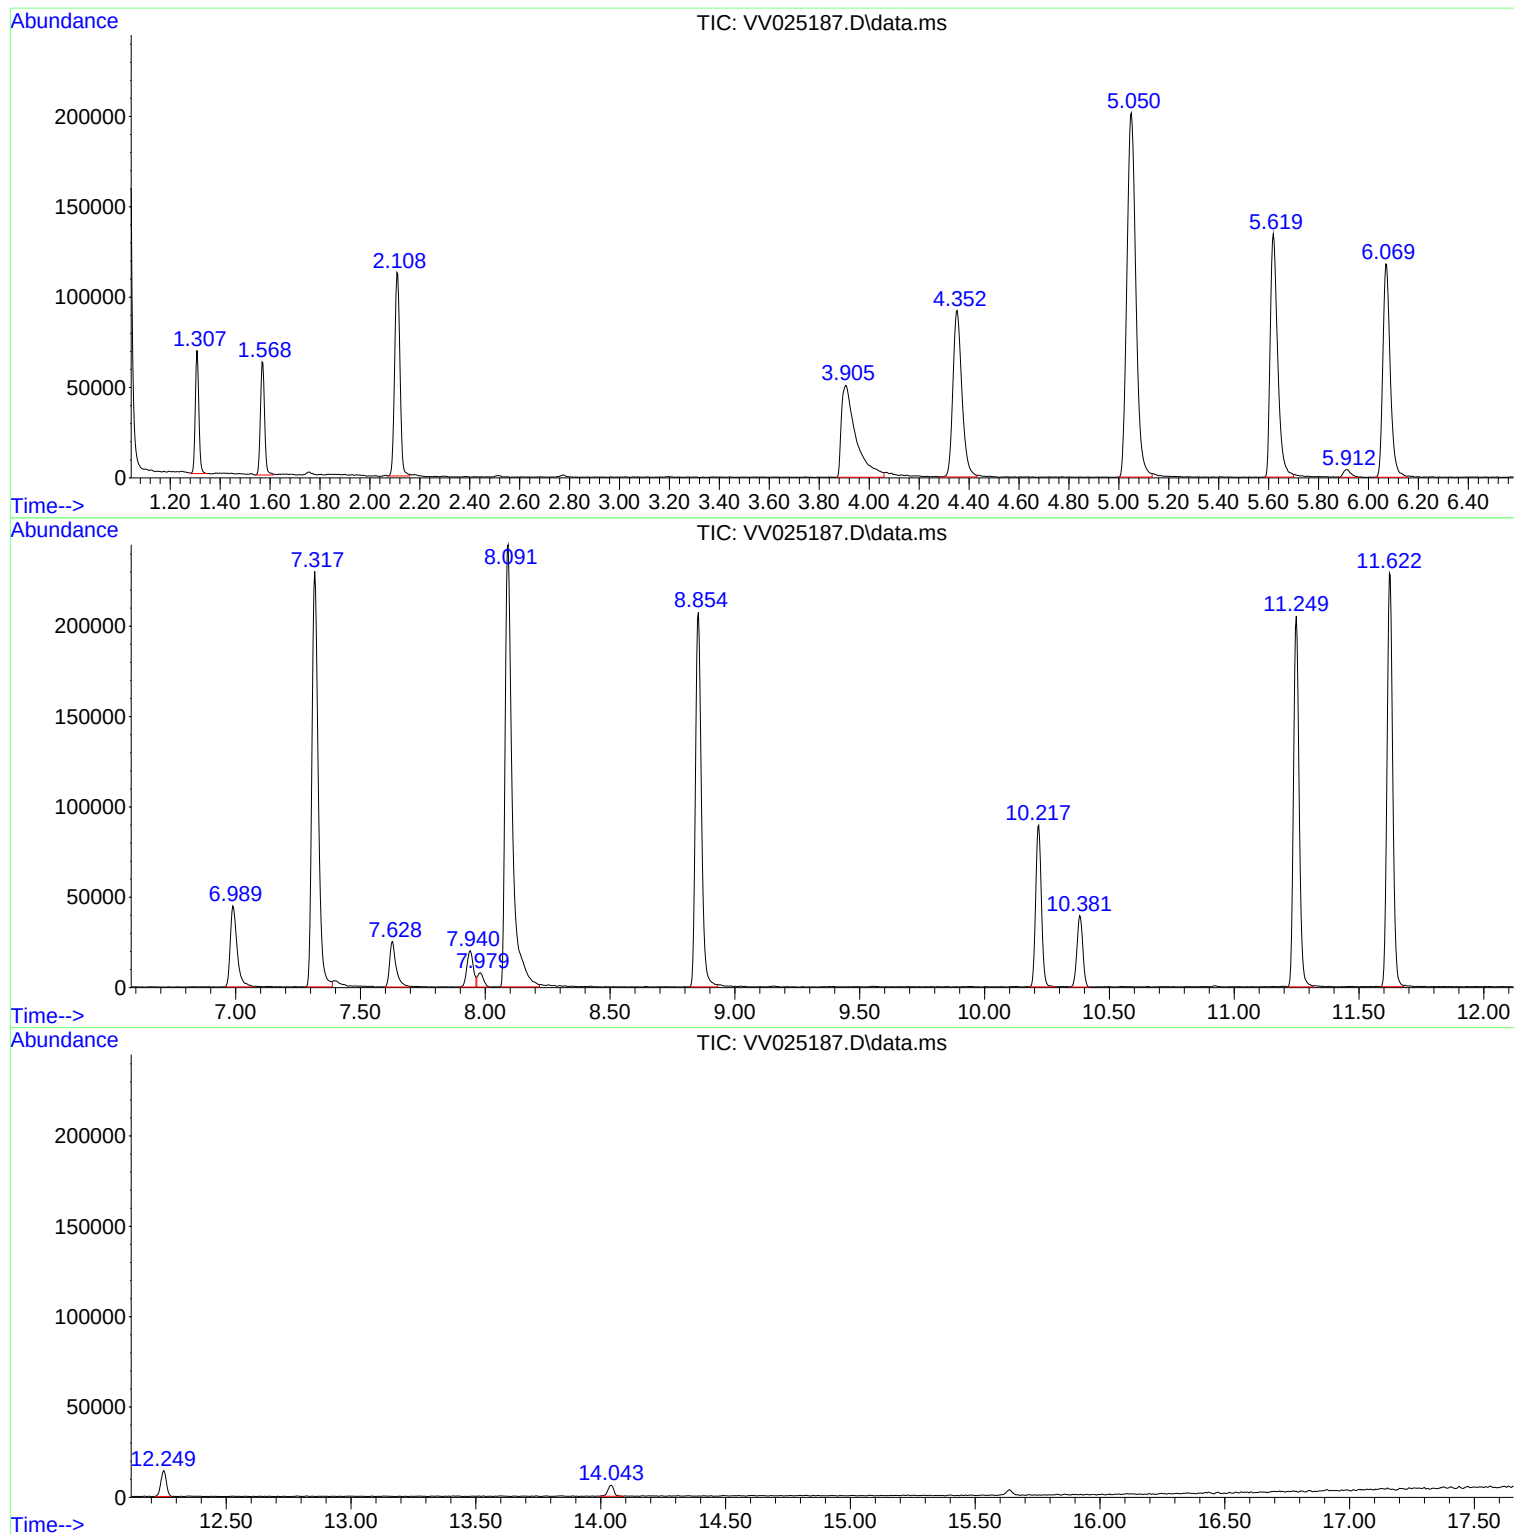

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032522\
Data File : VV025187.D
Acq On : 25 Mar 2022 18:50
Operator : SY/MD
Sample : N2097-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032522\
Data File : VV025187.D
Acq On : 25 Mar 2022 18:50
Operator : SY/MD
Sample : N2097-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
