




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025203.D
Acq On : 26 Mar 2022 17:12
Operator : SY/MD
Sample : N2083-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 03/28/2022
Supervised By :Mahesh Dadoda 03/28/2022

Quant Time: Mar 28 02:02:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Mar 28 01:44:37 2022
Response via : Initial Calibration

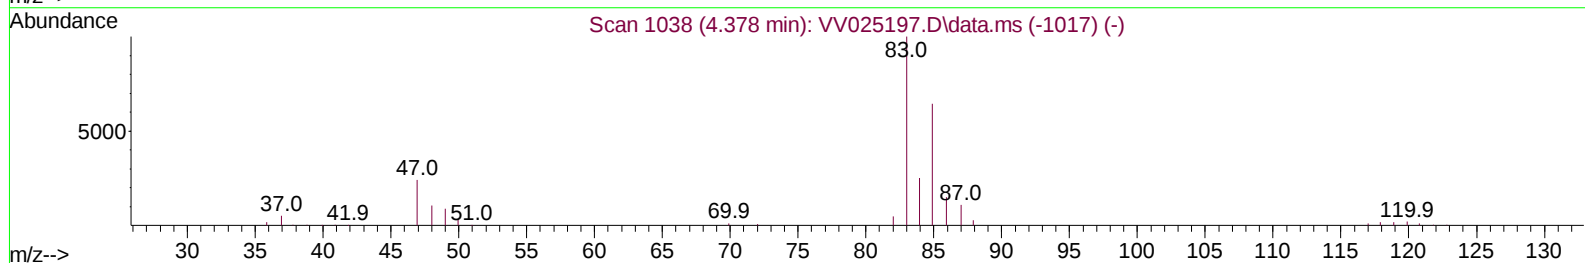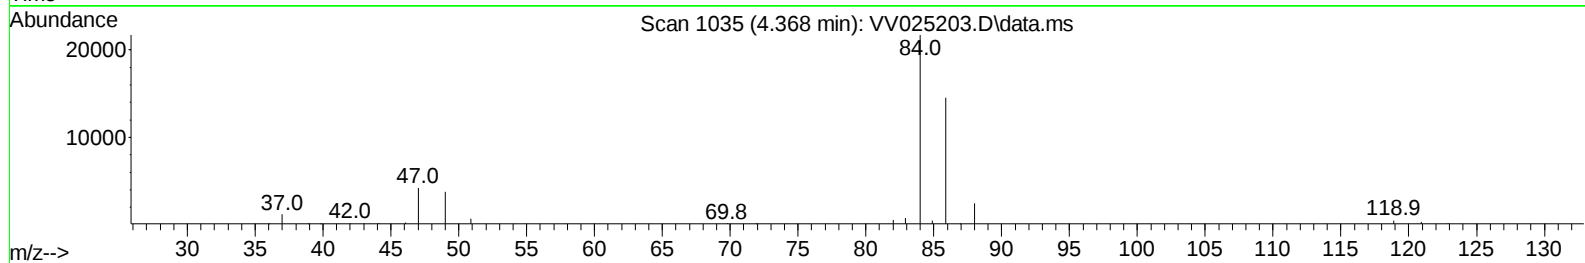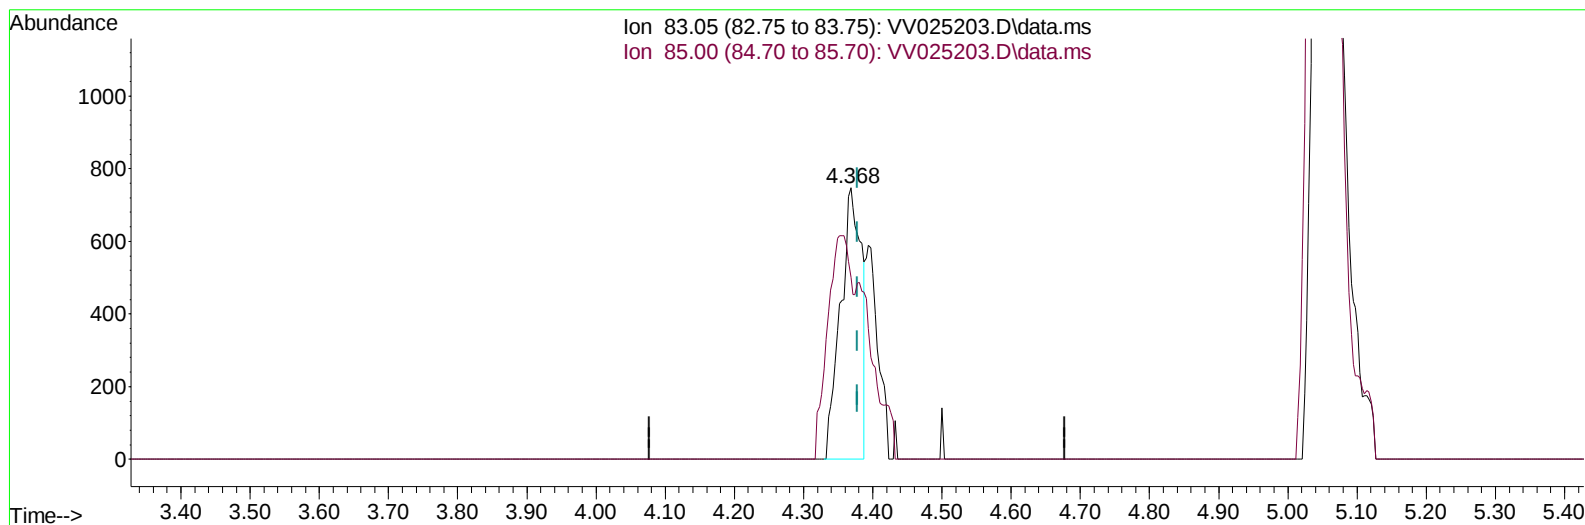

TIC: VV025203.D\data.ms

(25) Chloroform (T)

4.368min (-0.010) 0.08 ug/L

response 1567

Ion	Exp%	Act%
83.05	100.00	100.00
85.00	63.80	67.07
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025203.D
Acq On : 26 Mar 2022 17:12
Operator : SY/MD
Sample : N2083-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 03/28/2022
Supervised By :Mahesh Dadoda 03/28/2022

Quant Time: Mar 28 02:02:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Mar 28 01:44:37 2022
Response via : Initial Calibration

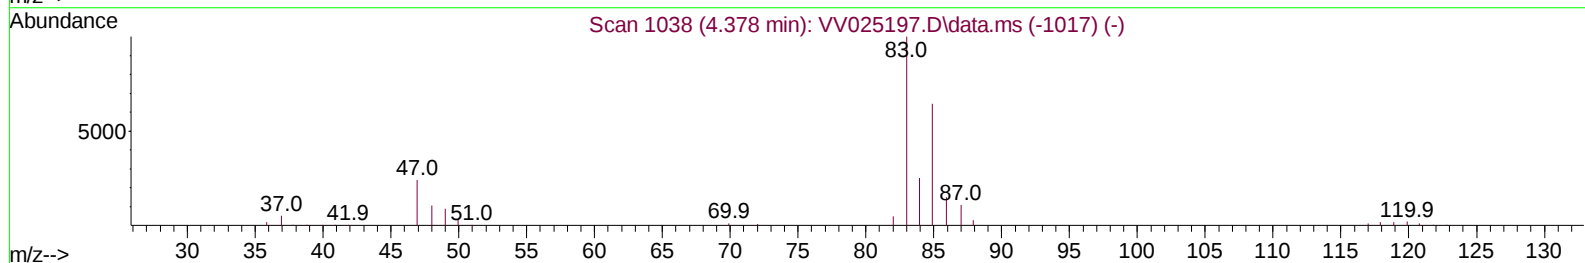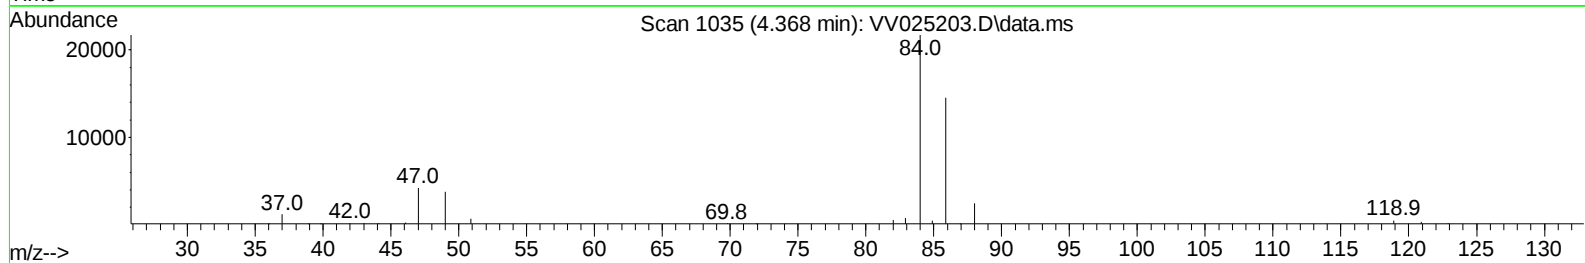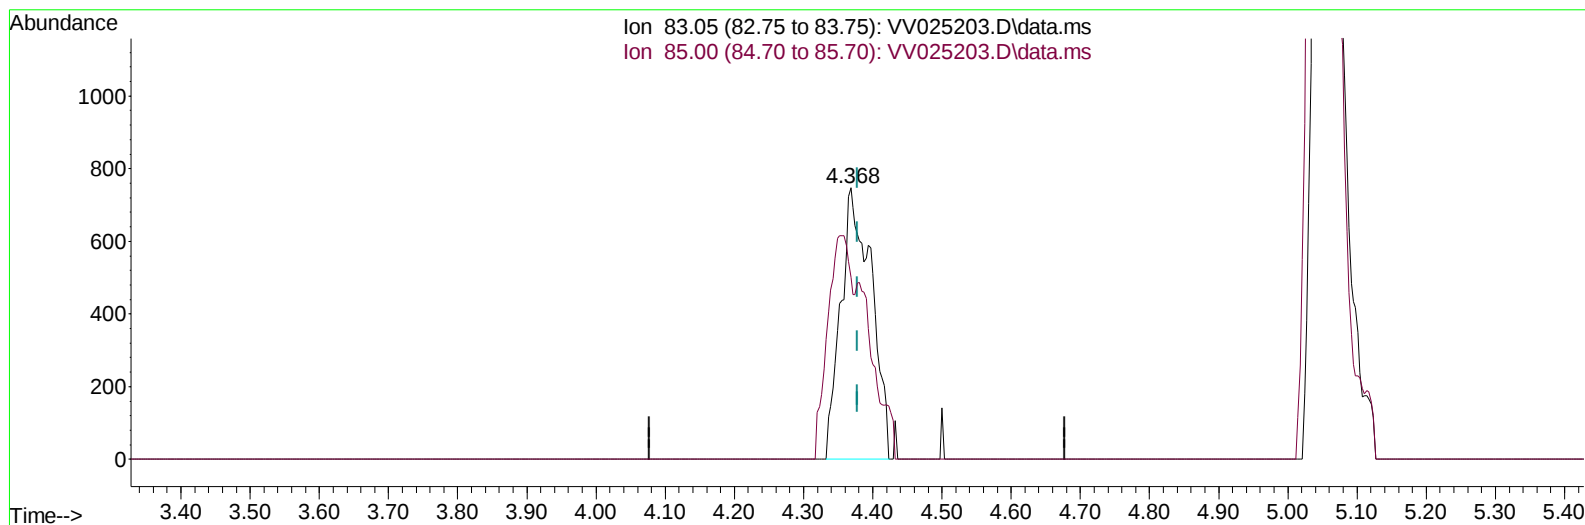

TIC: VV025203.D\data.ms

(25) Chloroform (T)

4.368min (-0.010) 0.12 ug/L m

response 2292

Ion	Exp%	Act%
83.05	100.00	100.00
85.00	63.80	67.07
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
 Data File : VV025203.D
 Acq On : 26 Mar 2022 17:12
 Operator : SY/MD
 Sample : N2083-15
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Mar 28 02:02:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Mar 28 01:44:37 2022
 Response via : Initial Calibration

Reviewed By : John Carlone 03/28/2022
 Supervised By : Mahesh Dadoda 03/28/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	147521	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	144528	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	62219	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	72392	5.253	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	105.000%	
7) Chloroethane-d5	1.568	69	62730	5.424	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	108.400%	
11) 1,1-Dichloroethene-d2	2.108	63	113187	3.792	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	75.800%	
20) 2-Butanone-d5	3.918	46	57048	41.561	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	83.120%	
24) Chloroform-d	4.352	84	92758	5.158	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	103.200%	
26) 1,2-Dichloroethane-d4	5.034	65	43698	5.498	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	110.000%	
32) Benzene-d6	5.050	84	193838	5.301	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	106.000%	
36) 1,2-Dichloropropane-d6	6.069	67	54403	5.309	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	106.200%	
41) Toluene-d8	7.316	98	166913	4.977	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	99.600%	
43) trans-1,3-Dichloroprop...	7.625	79	16721	5.002	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	100.000%	
46) 2-Hexanone-d5	8.091	63	60769	50.333	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	100.660%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	34629	5.068	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	101.400%	
66) 1,2-Dichlorobenzene-d4	11.625	152	54489	5.453	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	109.000%	
Target Compounds						
16) Methylene chloride	2.506	84	2749	0.236	ug/L	Qvalue 84
25) Chloroform	4.368	83	2292m	0.116	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025203.D
Acq On : 26 Mar 2022 17:12
Operator : SY/MD
Sample : N2083-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Mar 28 02:02:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Mar 28 01:44:37 2022
Response via : Initial Calibration

Reviewed By :John Carlone 03/28/2022
Supervised By :Mahesh Dadoda 03/28/2022

