




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
 Data File : VV025211.D
 Acq On : 26 Mar 2022 20:20
 Operator : SY/MD
 Sample : N2097-05
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD4

Manual IntegrationsAPPROVED

Quant Time: Mar 28 02:03:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Mar 28 01:44:37 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 03/28/2022
 Supervised By :Mahesh Dadoda 03/28/2022

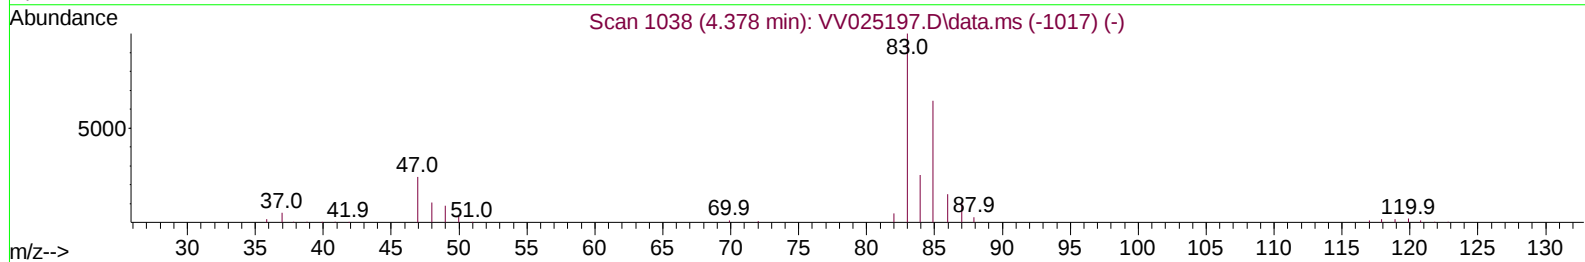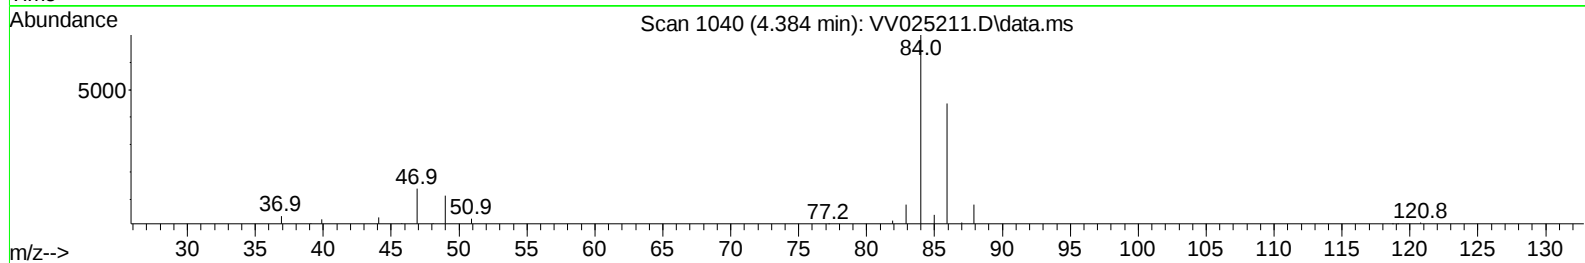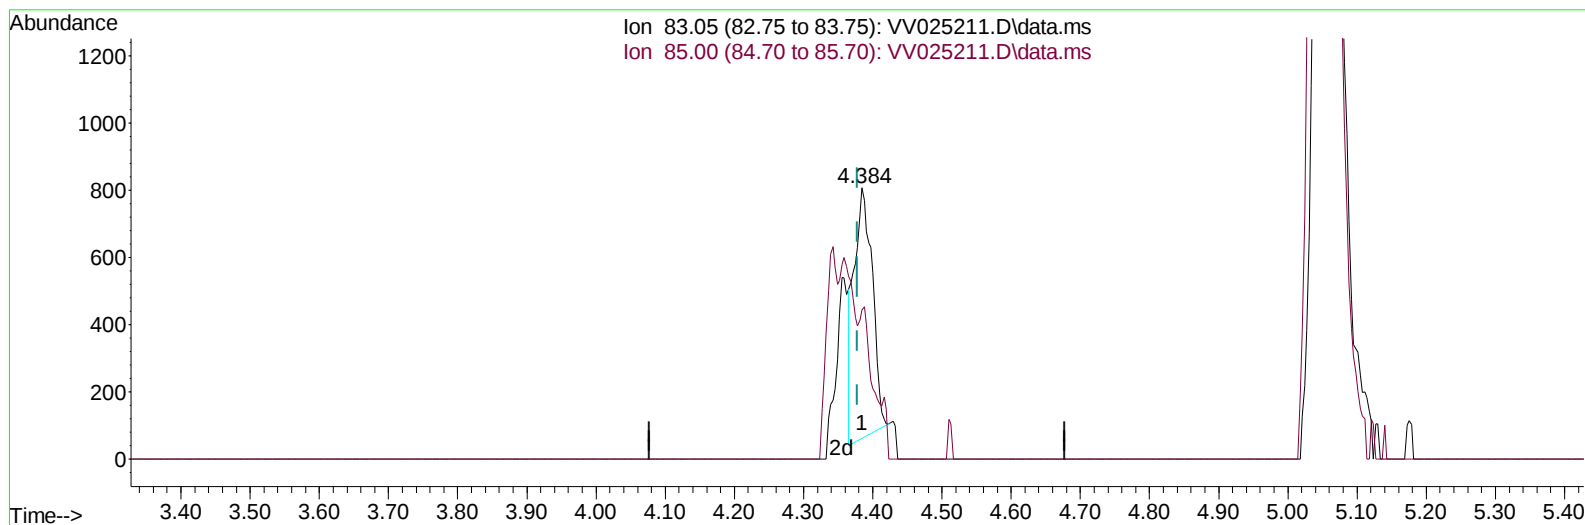

TIC: VV025211.D\data.ms

(25) Chloroform (T)

4.384min (+ 0.007) 0.07 ug/L

response 1382

Ion	Exp%	Act%
83.05	100.00	100.00
85.00	63.80	55.14
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025211.D
Acq On : 26 Mar 2022 20:20
Operator : SY/MD
Sample : N2097-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD4

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 03/28/2022
Supervised By :Mahesh Dadoda 03/28/2022

Quant Time: Mar 28 02:03:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Mar 28 01:44:37 2022
Response via : Initial Calibration

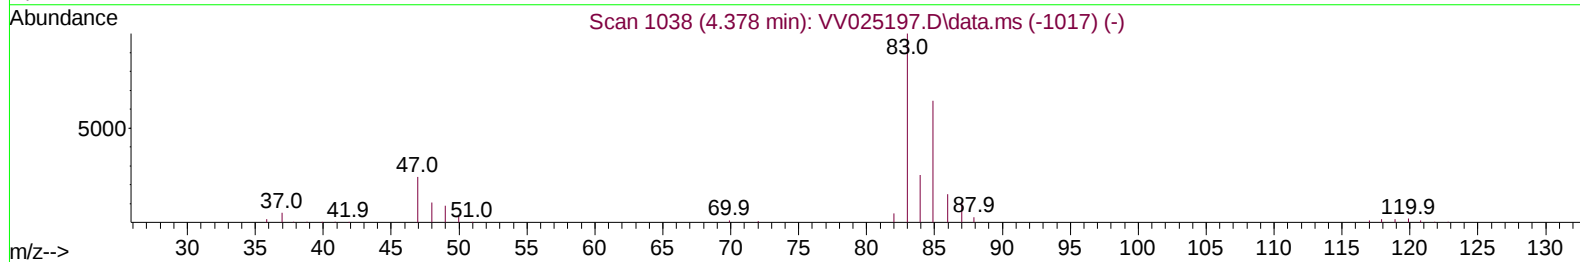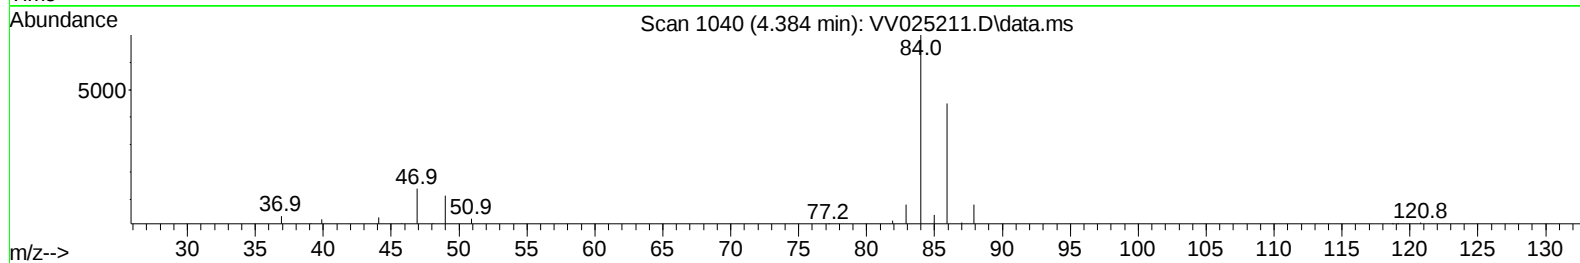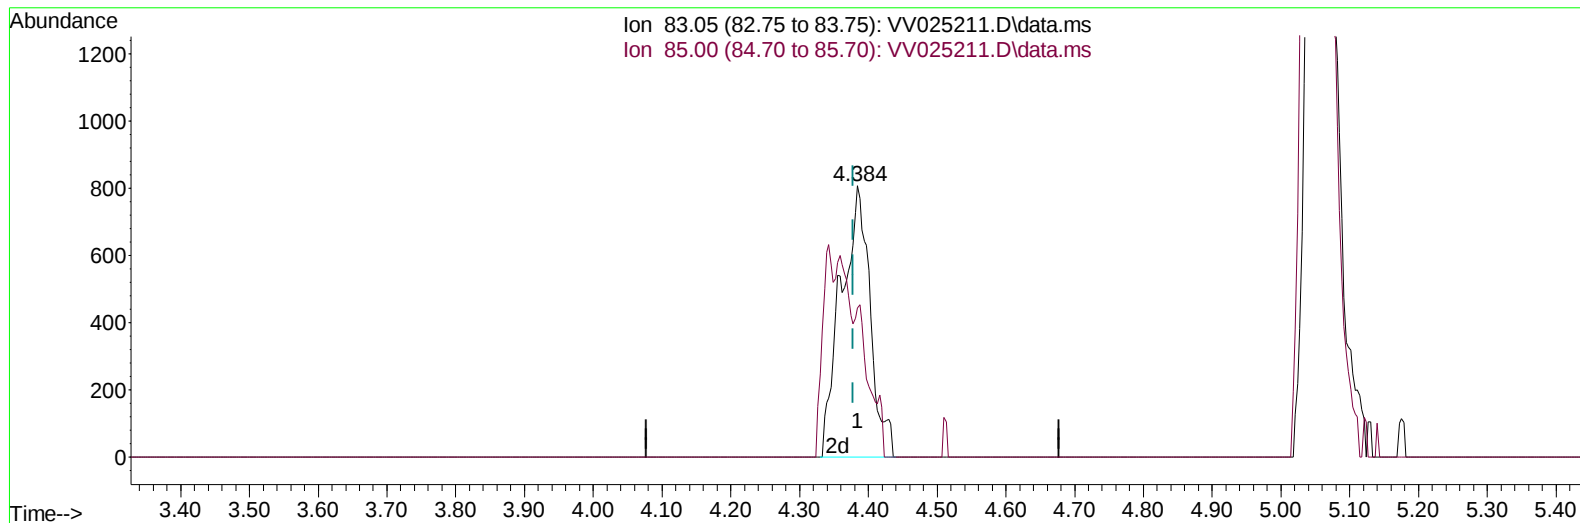

TIC: VV025211.D\data.ms

(25) Chloroform (T)

4.384min (+ 0.007) 0.12 ug/L m

response 2367

Ion	Exp%	Act%
83.05	100.00	100.00
85.00	63.80	55.14
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
 Data File : VV025211.D
 Acq On : 26 Mar 2022 20:20
 Operator : SY/MD
 Sample : N2097-05
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD4

Manual IntegrationsAPPROVED

Quant Time: Mar 28 02:03:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Mar 28 01:44:37 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 03/28/2022
 Supervised By :Mahesh Dadoda 03/28/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	149216	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	144808	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	63699	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	64520	4.629	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	92.600%	
7) Chloroethane-d5	1.568	69	56635	4.841	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	96.800%	
11) 1,1-Dichloroethene-d2	2.108	63	99653	3.301	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	66.000%	
20) 2-Butanone-d5	3.905	46	66435	47.850	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	95.700%	
24) Chloroform-d	4.352	84	90894	4.997	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	100.000%	
26) 1,2-Dichloroethane-d4	5.034	65	42634	5.303	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	106.000%	
32) Benzene-d6	5.050	84	183602	5.012	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	100.200%	
36) 1,2-Dichloropropane-d6	6.069	67	53122	5.174	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	103.400%	
41) Toluene-d8	7.317	98	160839	4.787	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	95.800%	
43) trans-1,3-Dichloroprop...	7.625	79	15403	4.599	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	92.000%	
46) 2-Hexanone-d5	8.088	63	56430	46.648	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	93.300%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	32780	4.788	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	95.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	53720	5.251	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	105.000%	
Target Compounds						Qvalue
25) Chloroform	4.384	83	2367m	0.119	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025211.D
Acq On : 26 Mar 2022 20:20
Operator : SY/MD
Sample : N2097-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD4

Manual IntegrationsAPPROVED

Quant Time: Mar 28 02:03:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Mar 28 01:44:37 2022
Response via : Initial Calibration

Reviewed By :John Carlone 03/28/2022
Supervised By :Mahesh Dadoda 03/28/2022

