




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
 Data File : VV025230.D
 Acq On : 27 Mar 2022 04:08
 Operator : SY/MD
 Sample : N2110-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0PB2

Manual IntegrationsAPPROVED

Quant Time: Mar 28 03:48:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Mar 28 03:13:34 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 03/28/2022
 Supervised By :Mahesh Dadoda 03/28/2022

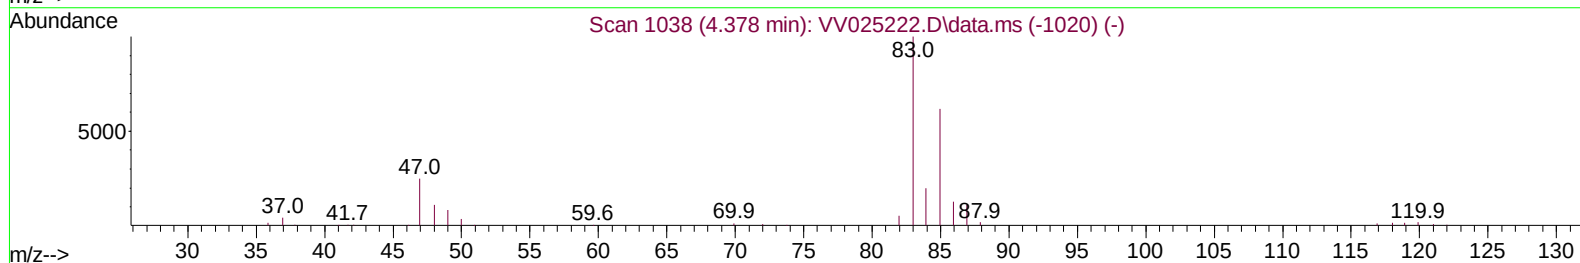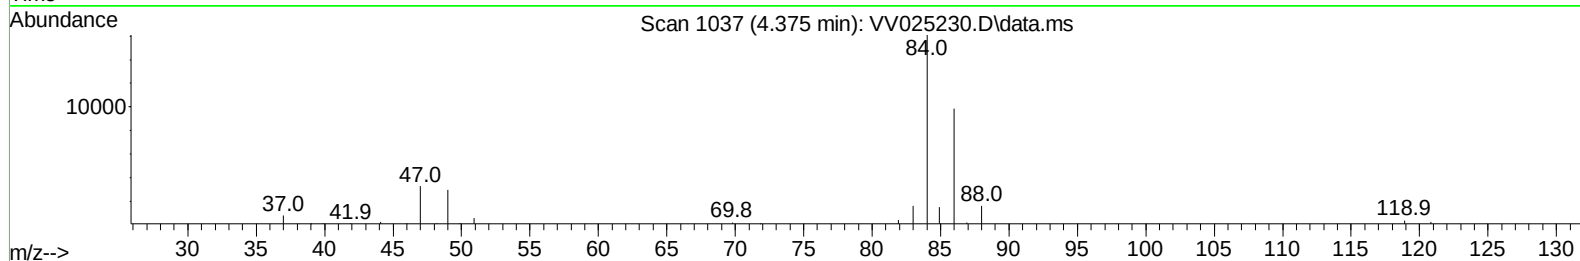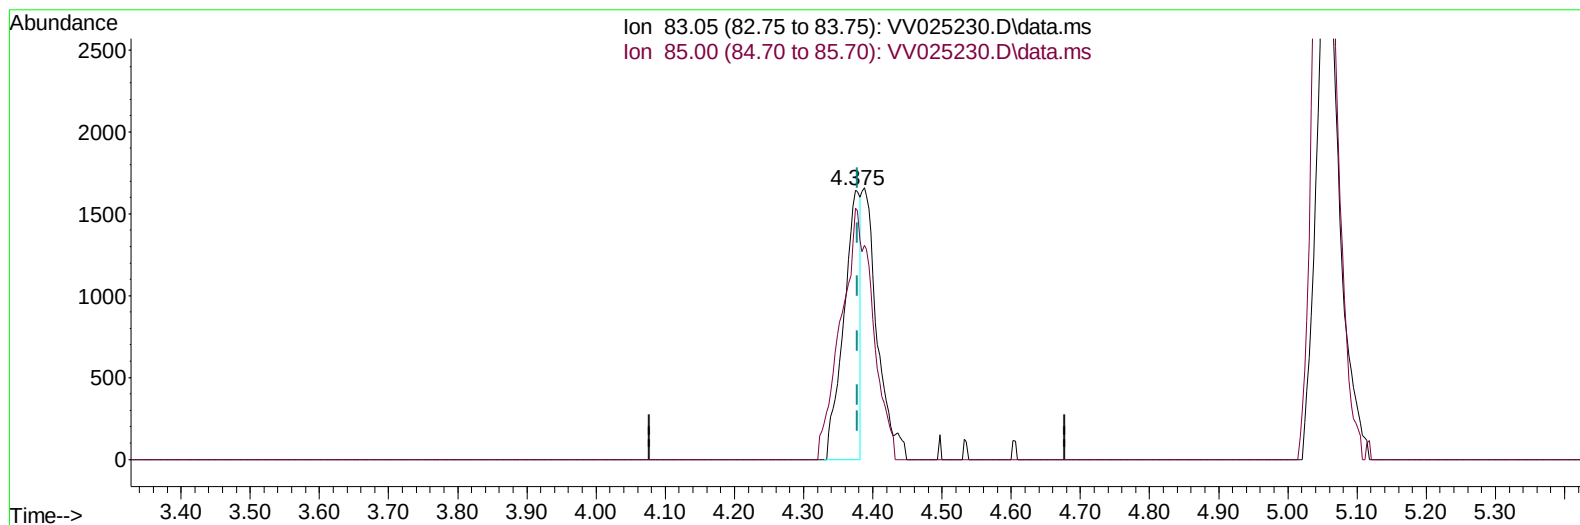

TIC: VV025230.D\data.ms

(25) Chloroform (T)

4.375min (-0.003) 0.13 ug/L

response 2673

Ion	Exp%	Act%
83.05	100.00	100.00
85.00	63.80	93.37#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025230.D
Acq On : 27 Mar 2022 04:08
Operator : SY/MD
Sample : N2110-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PB2

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 03/28/2022
Supervised By :Mahesh Dadoda 03/28/2022

Quant Time: Mar 28 03:48:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Mar 28 03:13:34 2022
Response via : Initial Calibration

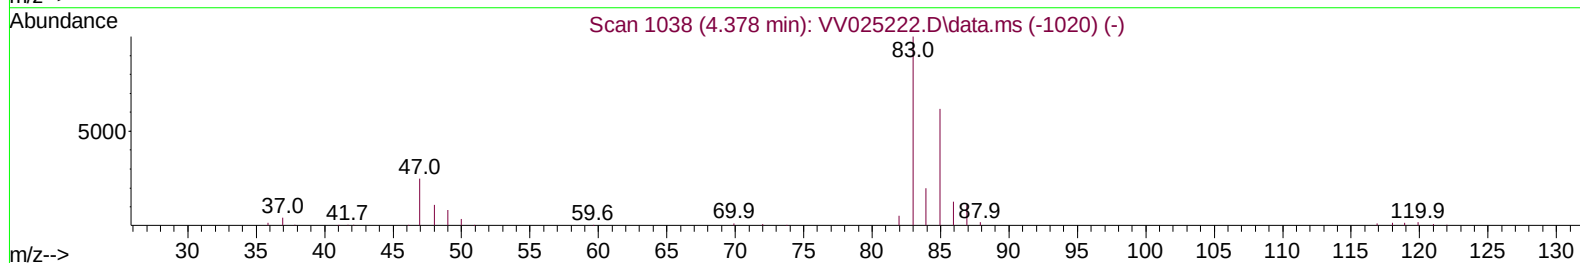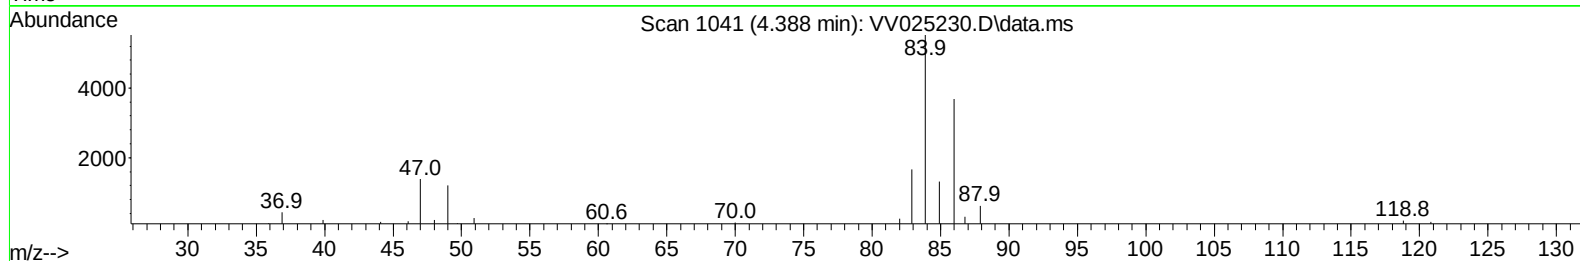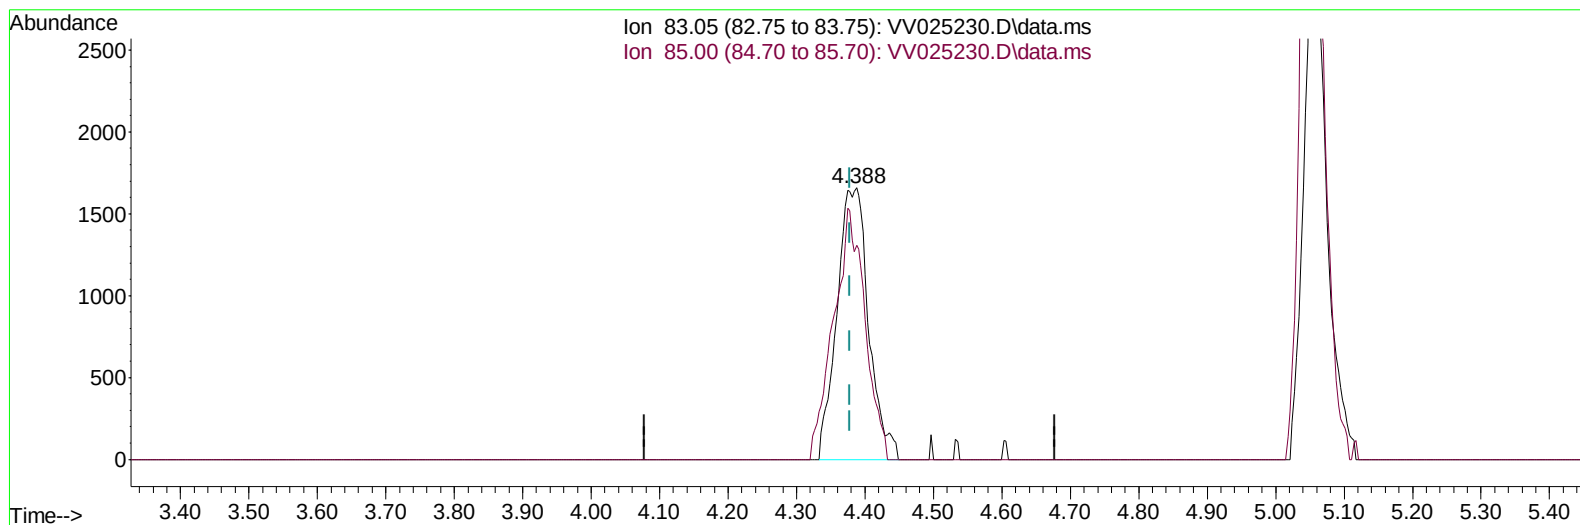

TIC: VV025230.D\data.ms

(25) Chloroform (T)

4.388min (+ 0.010) 0.27 ug/L m

response 5324

Ion	Exp%	Act%
83.05	100.00	100.00
85.00	63.80	78.83
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
 Data File : VV025230.D
 Acq On : 27 Mar 2022 04:08
 Operator : SY/MD
 Sample : N2110-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0PB2

Manual IntegrationsAPPROVED

Quant Time: Mar 28 03:48:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Mar 28 03:13:34 2022
 Response via : Initial Calibration

Reviewed By : John Carlone 03/28/2022
 Supervised By : Mahesh Dadoda 03/28/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	149520	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	145556	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	61604	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	60318	4.319	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	86.400%		
7) Chloroethane-d5	1.571	69	54008	4.607	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	92.200%		
11) 1,1-Dichloroethene-d2	2.111	63	97225	3.214	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	64.200%		
20) 2-Butanone-d5	3.908	46	70602	50.748	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	101.500%		
24) Chloroform-d	4.352	84	90845	4.984	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	99.600%		
26) 1,2-Dichloroethane-d4	5.037	65	40749	5.058	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	101.200%		
32) Benzene-d6	5.053	84	181330	4.924	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	98.400%		
36) 1,2-Dichloropropane-d6	6.069	67	51730	5.013	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	100.200%		
41) Toluene-d8	7.317	98	158439	4.691	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	93.800%		
43) trans-1,3-Dichloroprop...	7.625	79	14864	4.415	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	88.200%		
46) 2-Hexanone-d5	8.088	63	65480	53.852	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	107.700%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	33183	4.822	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	96.400%		
66) 1,2-Dichlorobenzene-d4	11.625	152	53759	5.433	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	108.600%		
Target Compounds						
25) Chloroform	4.388	83	5324m	0.266	ug/L	
47) Tetrachloroethene	7.973	164	1040520	120.363	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025230.D
Acq On : 27 Mar 2022 04:08
Operator : SY/MD
Sample : N2110-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PB2

Manual IntegrationsAPPROVED

Quant Time: Mar 28 03:48:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Mar 28 03:13:34 2022
Response via : Initial Calibration

Reviewed By :John Carlone 03/28/2022
Supervised By :Mahesh Dadoda 03/28/2022

