




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025234.D
Acq On : 27 Mar 2022 05:41
Operator : SY/MD
Sample : N2110-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PB6

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 03/28/2022
Supervised By :Mahesh Dadoda 03/28/2022

Quant Time: Mar 28 03:49:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Mar 28 03:13:34 2022
Response via : Initial Calibration

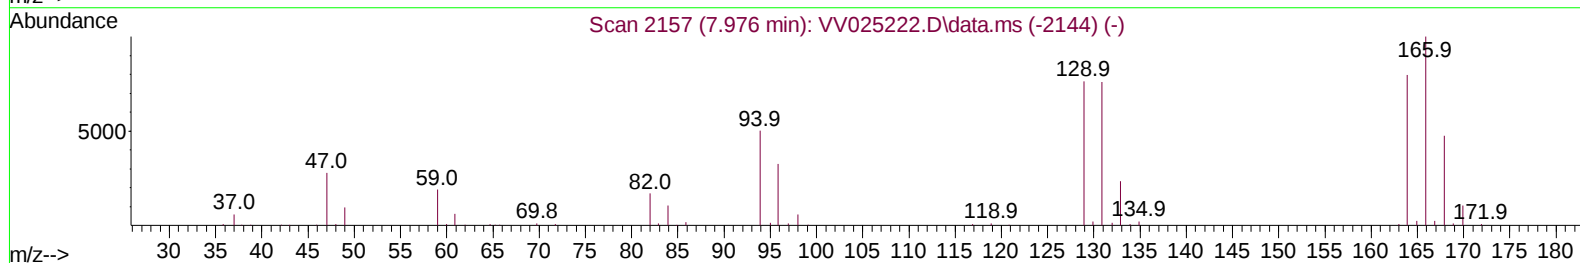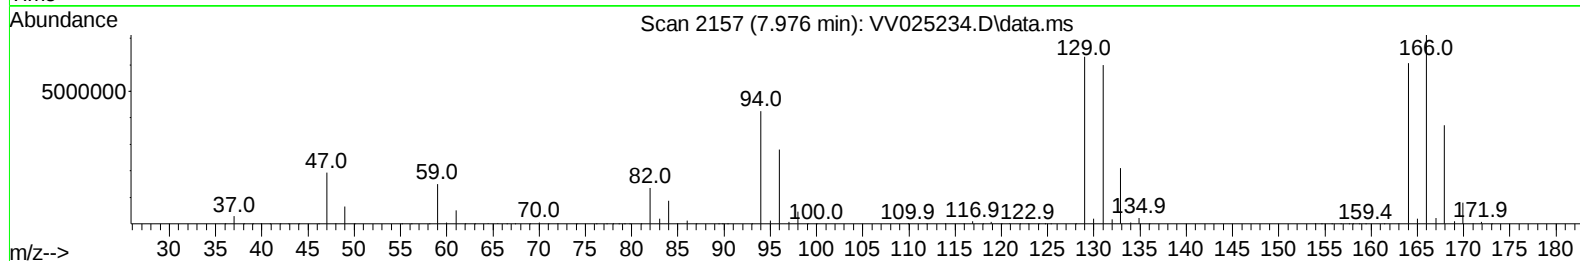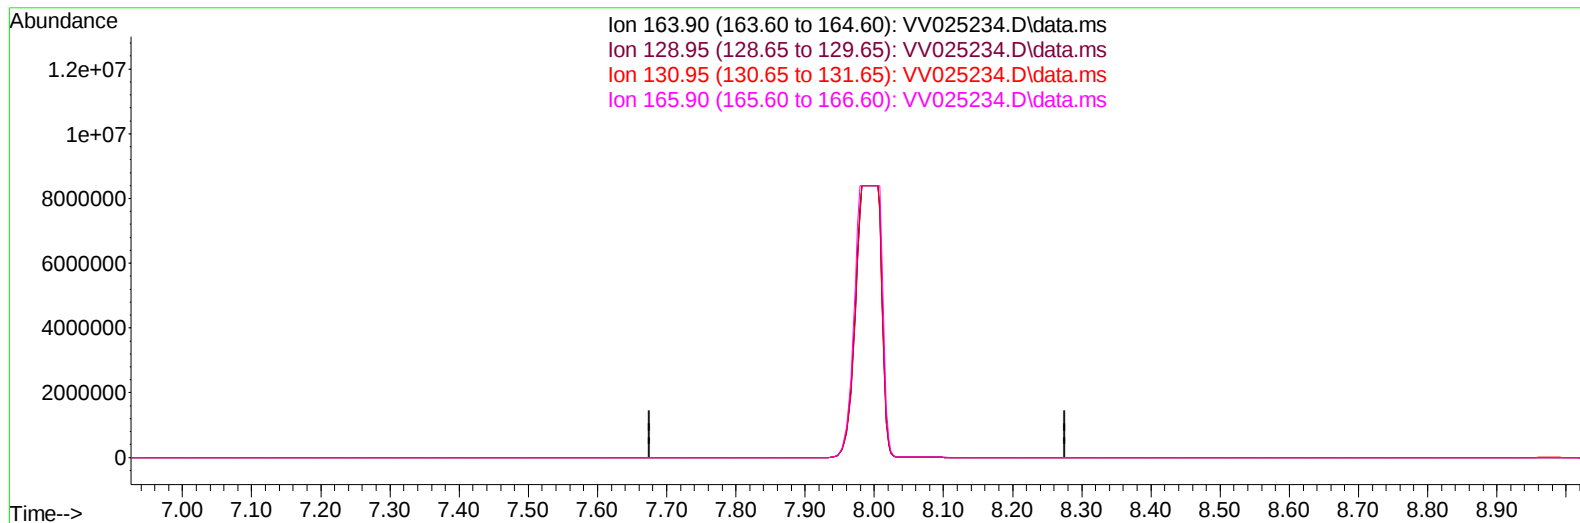

TIC: VV025234.D\data.ms

(47) Tetrachloroethene (T)

7.976min (-7.976) 0.00 ug/L

response 0

Ion	Exp%	Act%
163.90	100.00	0.00
128.95	96.50	0.00#
130.95	97.20	0.00#
165.90	123.20	0.00#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
 Data File : VV025234.D
 Acq On : 27 Mar 2022 05:41
 Operator : SY/MD
 Sample : N2110-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0PB6

Manual IntegrationsAPPROVED

Quant Time: Mar 28 03:49:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Mar 28 03:13:34 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 03/28/2022
 Supervised By :Mahesh Dadoda 03/28/2022

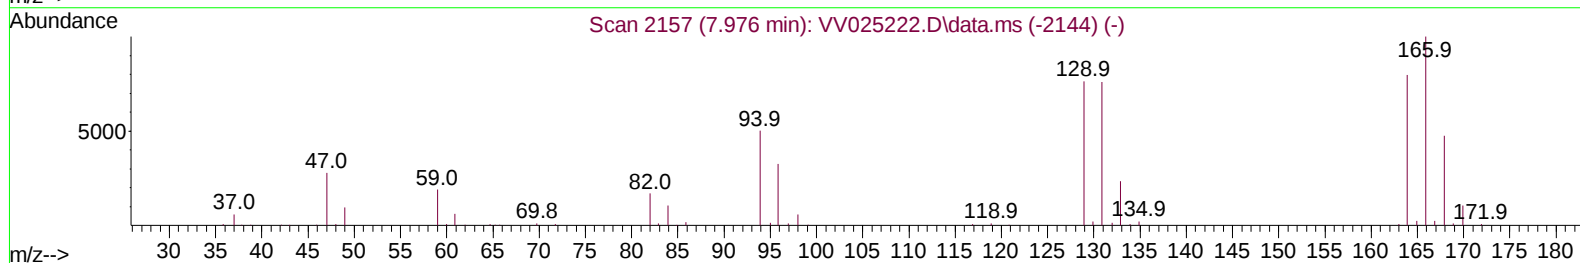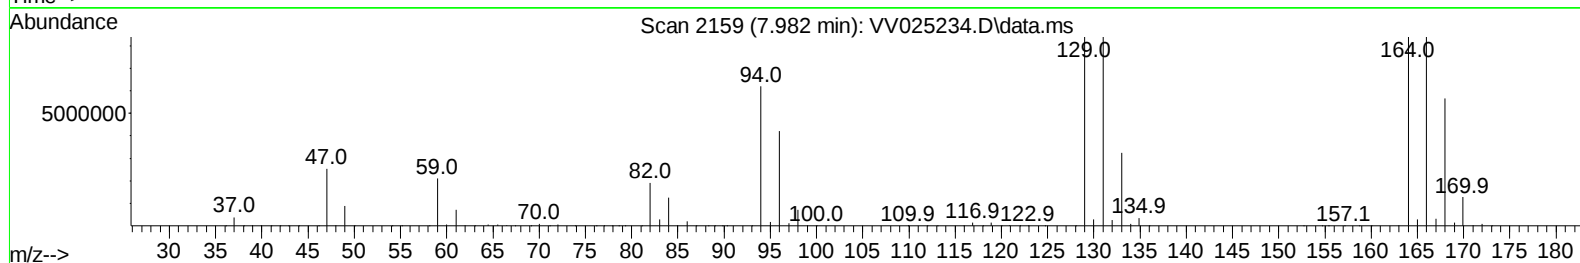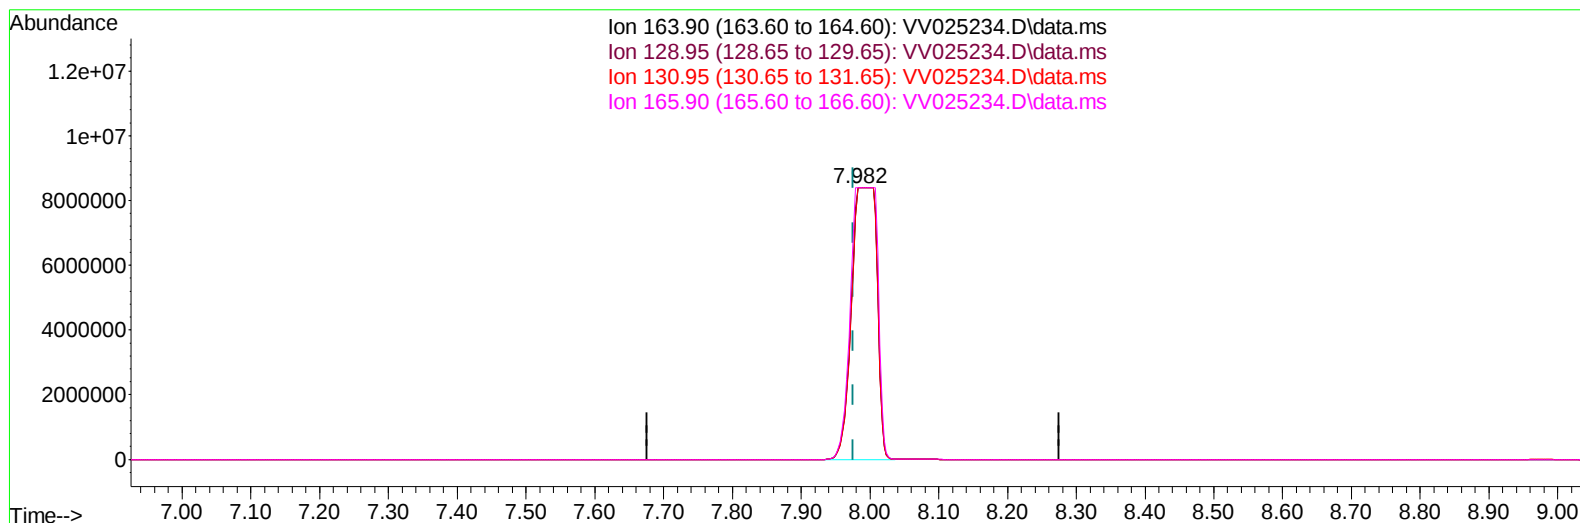

TIC: VV025234.D\data.ms

(47) Tetrachloroethene (T)

7.982min (+ 0.007) 2640.41 ug/L m

response 21429288

Ion	Exp%	Act%
163.90	100.00	100.00
128.95	96.50	100.00
130.95	97.20	100.00
165.90	123.20	100.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
 Data File : VV025234.D
 Acq On : 27 Mar 2022 05:41
 Operator : SY/MD
 Sample : N2110-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0PB6

Manual IntegrationsAPPROVED

Quant Time: Mar 28 03:49:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Mar 28 03:13:34 2022
 Response via : Initial Calibration

Reviewed By : John Carlone 03/28/2022
 Supervised By : Mahesh Dadoda 03/28/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	145602	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	136650	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	59020	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	60868	4.475	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	89.600%	
7) Chloroethane-d5	1.571	69	55264	4.841	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	96.800%	
11) 1,1-Dichloroethene-d2	2.111	63	99524	3.378	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	67.600%	
20) 2-Butanone-d5	3.912	46	63379	46.782	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	93.560%	
24) Chloroform-d	4.349	84	89615	5.049	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	101.000%	
26) 1,2-Dichloroethane-d4	5.037	65	41293	5.263	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	105.200%	
32) Benzene-d6	5.053	84	180983	5.235	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	104.800%	
36) 1,2-Dichloropropane-d6	6.072	67	52099	5.377	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	107.600%	
41) Toluene-d8	7.317	98	156223	4.927	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	98.600%	
43) trans-1,3-Dichloroprop...	7.625	79	14916	4.719	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	94.400%	
46) 2-Hexanone-d5	8.088	63	66639	58.377	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	116.760%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	32035	4.959	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	99.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	52880	5.579	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	111.600%	
Target Compounds						
					Qvalue	
12) 1,1-Dichloroethene	2.114	96	1943	0.133	ug/L #	1
17) Methyl tert-butyl Ether	2.774	73	11463	0.618	ug/L #	90
18) trans-1,2-Dichloroethene	2.767	96	648	0.062	ug/L	81
22) cis-1,2-Dichloroethene	3.915	96	25417	2.378	ug/L	100
25) Chloroform	4.378	83	9044	0.464	ug/L	95
34) Trichloroethene	5.918	95	34372	3.123	ug/L	98
47) Tetrachloroethene	7.982	164	21429288m	2640.408	ug/L	
51) Chlorobenzene	8.883	112	2439	0.088	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025234.D
Acq On : 27 Mar 2022 05:41
Operator : SY/MD
Sample : N2110-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PB6

Manual IntegrationsAPPROVED

Quant Time: Mar 28 03:49:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Mar 28 03:13:34 2022
Response via : Initial Calibration

Reviewed By :John Carlone 03/28/2022
Supervised By :Mahesh Dadoda 03/28/2022

