




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
 Data File : VV025239.D
 Acq On : 27 Mar 2022 07:38
 Operator : SY/MD
 Sample : N2110-11
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0PC7

Manual IntegrationsAPPROVED

Quant Time: Mar 28 04:36:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Mar 28 03:13:34 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 03/28/2022
 Supervised By :Mahesh Dadoda 03/28/2022

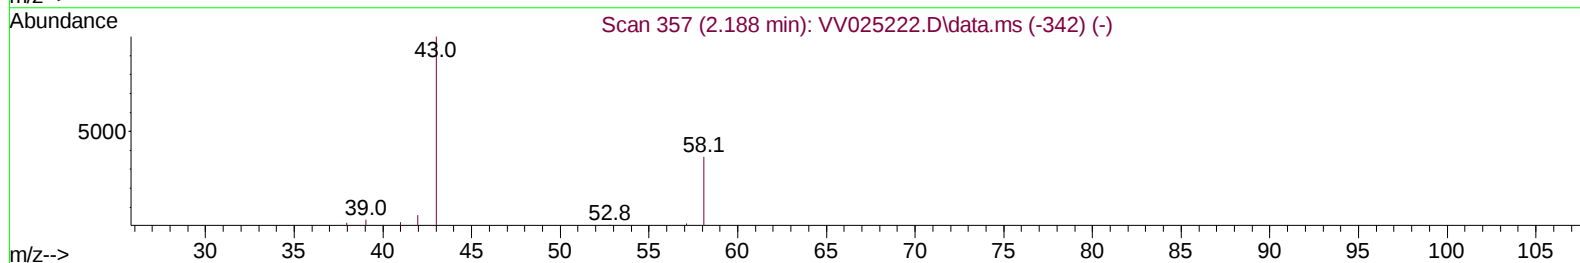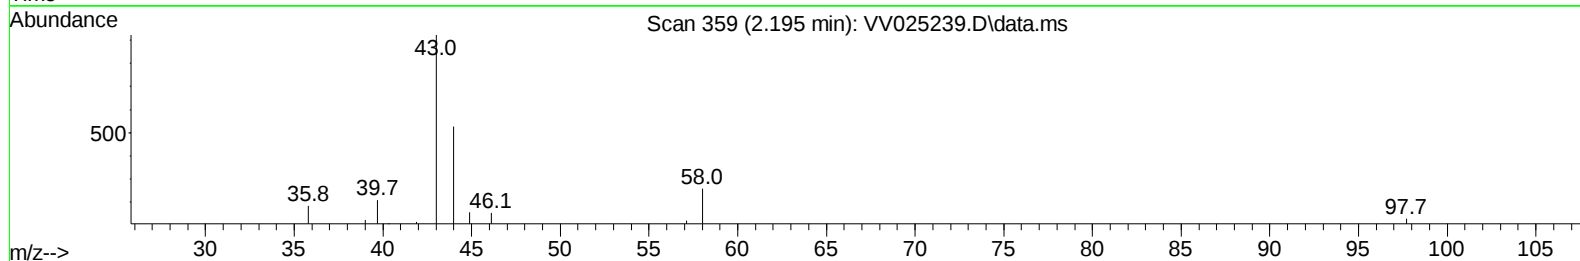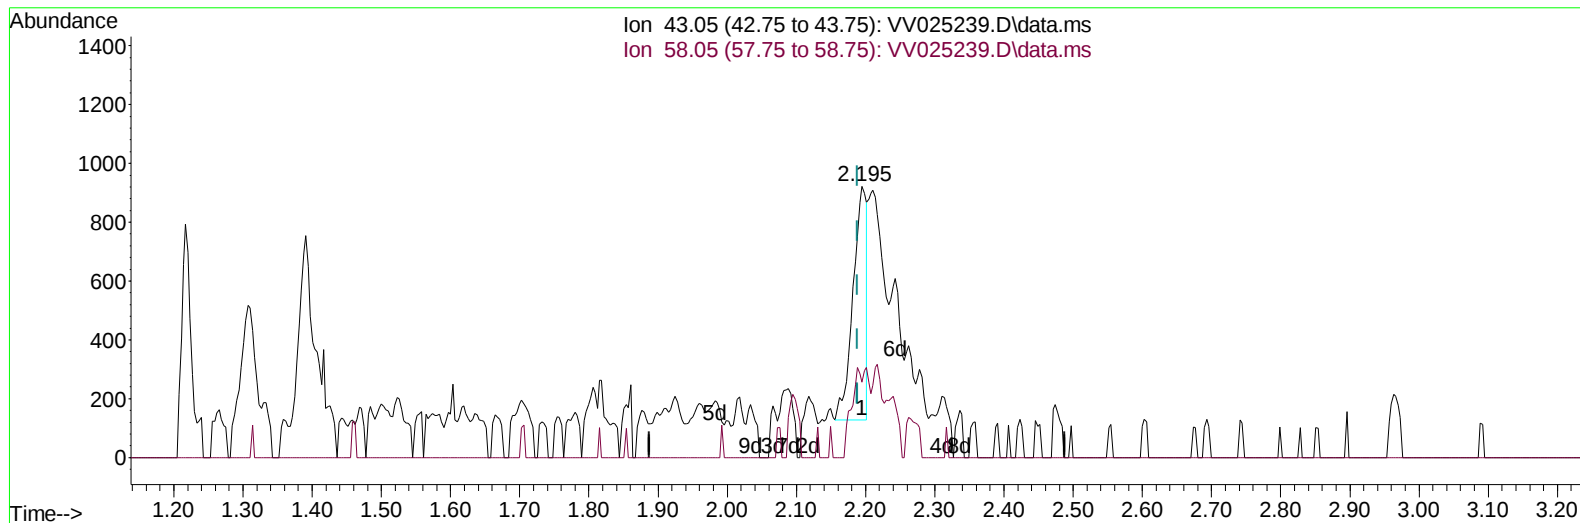

TIC: VV025239.D\data.ms

(13) Acetone (T)

2.195min (+ 0.007) 1.06 ug/L

response 1083

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	25.60	30.38
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
 Data File : VV025239.D
 Acq On : 27 Mar 2022 07:38
 Operator : SY/MD
 Sample : N2110-11
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0PC7

Manual IntegrationsAPPROVED

Quant Time: Mar 28 04:36:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Mar 28 03:13:34 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 03/28/2022
 Supervised By :Mahesh Dadoda 03/28/2022

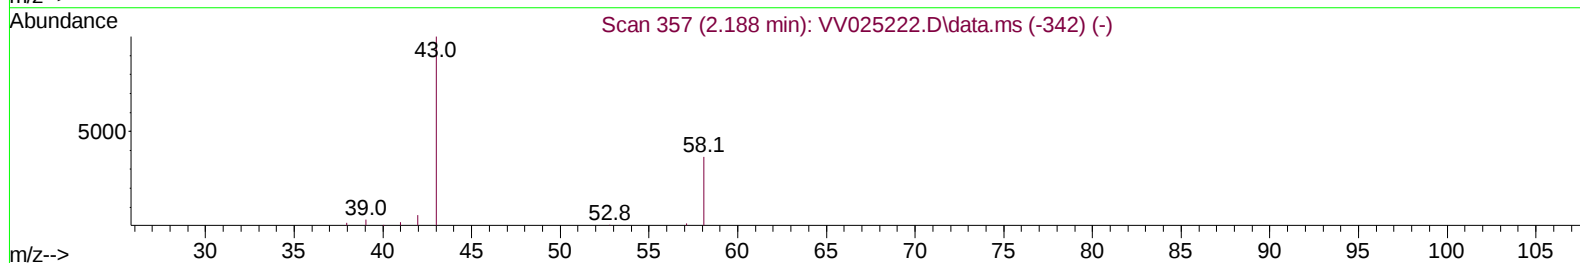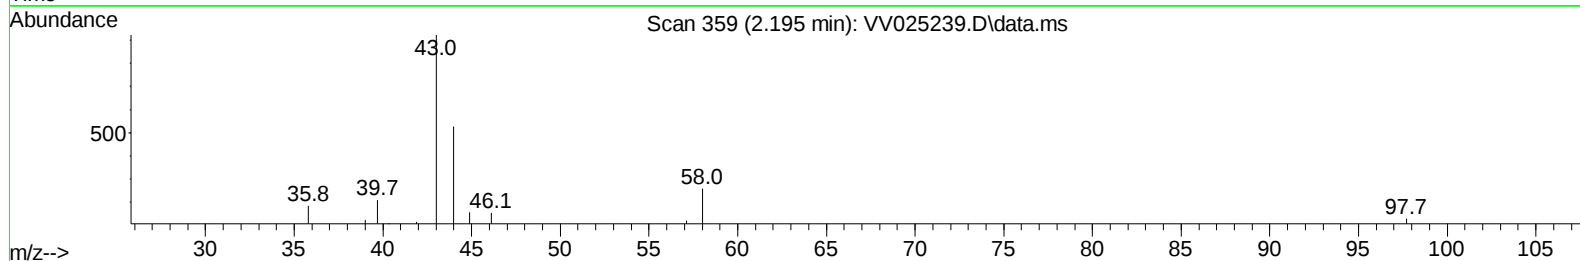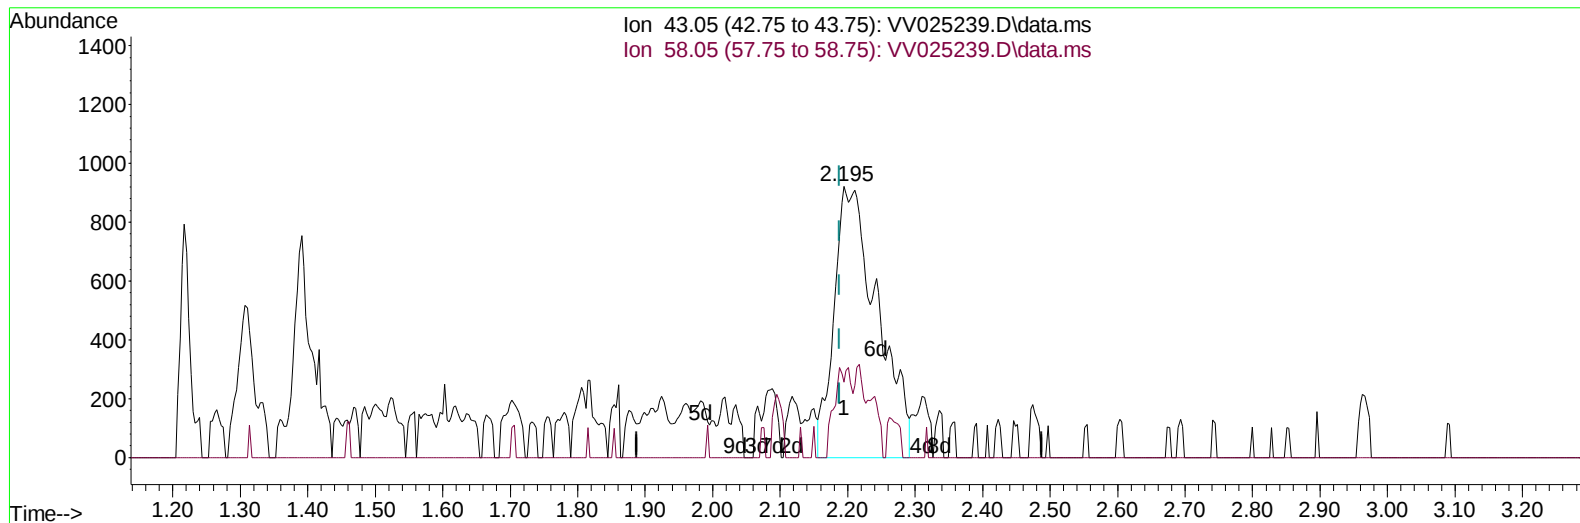

TIC: VV025239.D\data.ms

(13) Acetone (T)

2.195min (+ 0.007) 4.00 ug/L m

response 4097

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	25.60	8.03
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
 Data File : VV025239.D
 Acq On : 27 Mar 2022 07:38
 Operator : SY/MD
 Sample : N2110-11
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0PC7

Manual IntegrationsAPPROVED

Quant Time: Mar 28 04:36:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Mar 28 03:13:34 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 03/28/2022
 Supervised By :Mahesh Dadoda 03/28/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	144195	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	139802	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	57882	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	61141	4.539	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	90.800%		
7) Chloroethane-d5	1.571	69	54305	4.804	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	96.000%		
11) 1,1-Dichloroethene-d2	2.111	63	97887	3.355	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	67.200%		
20) 2-Butanone-d5	3.905	46	64566	48.124	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	96.240%		
24) Chloroform-d	4.352	84	95708	5.445	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	108.800%		
26) 1,2-Dichloroethane-d4	5.034	65	42402	5.458	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	109.200%		
32) Benzene-d6	5.053	84	180129	5.093	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	101.800%		
36) 1,2-Dichloropropane-d6	6.072	67	52496	5.296	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	106.000%		
41) Toluene-d8	7.317	98	158489	4.885	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	97.800%		
43) trans-1,3-Dichloroprop...	7.625	79	14241	4.404	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	88.000%		
46) 2-Hexanone-d5	8.088	63	56645	48.503	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	97.000%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	33116	5.011	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	100.200%		
66) 1,2-Dichlorobenzene-d4	11.622	152	55449	5.965	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	119.200%		
Target Compounds						
					Qvalue	
13) Acetone	2.195	43	4097m	4.002	ug/L	
25) Chloroform	4.378	83	129515	6.711	ug/L	99
38) Bromodichloromethane	6.513	83	14474	1.201	ug/L	94
47) Tetrachloroethene	7.976	164	13113	1.579	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025239.D
Acq On : 27 Mar 2022 07:38
Operator : SY/MD
Sample : N2110-11
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PC7

Manual IntegrationsAPPROVED

Quant Time: Mar 28 04:36:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Mar 28 03:13:34 2022
Response via : Initial Calibration

Reviewed By :John Carlone 03/28/2022
Supervised By :Mahesh Dadoda 03/28/2022

