

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032622\
 Data File : VW025213.D
 Acq On : 26 Mar 2022 21:07
 Operator : SY/MD
 Sample : N2097-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD6

Quant Time: Mar 28 02:04:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Mar 28 01:44:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	153566	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	151841	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	64281	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	66485	4.635	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.600%
7) Chloroethane-d5	1.568	69	57363	4.765	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.200%
11) 1,1-Dichloroethene-d2	2.108	63	104677	3.369	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.400%
20) 2-Butanone-d5	3.918	46	68304	47.803	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.600%
24) Chloroform-d	4.352	84	92131	4.922	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.400%
26) 1,2-Dichloroethane-d4	5.034	65	42890	5.184	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.600%
32) Benzene-d6	5.053	84	185525	4.830	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.600%
36) 1,2-Dichloropropane-d6	6.069	67	53354	4.956	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.200%
41) Toluene-d8	7.317	98	163353	4.636	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.800%
43) trans-1,3-Dichloroprop...	7.625	79	14975	4.264	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.200%
46) 2-Hexanone-d5	8.091	63	60136	47.409	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.820%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	33872	4.719	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	54954	5.323	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.400%
Target Compounds						Qvalue
47) Tetrachloroethene	7.979	164	8287	0.919	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025213.D
Acq On : 26 Mar 2022 21:07
Operator : SY/MD
Sample : N2097-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD6


Quant Time: Mar 28 02:04:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Mar 28 01:44:37 2022
Response via : Initial Calibration

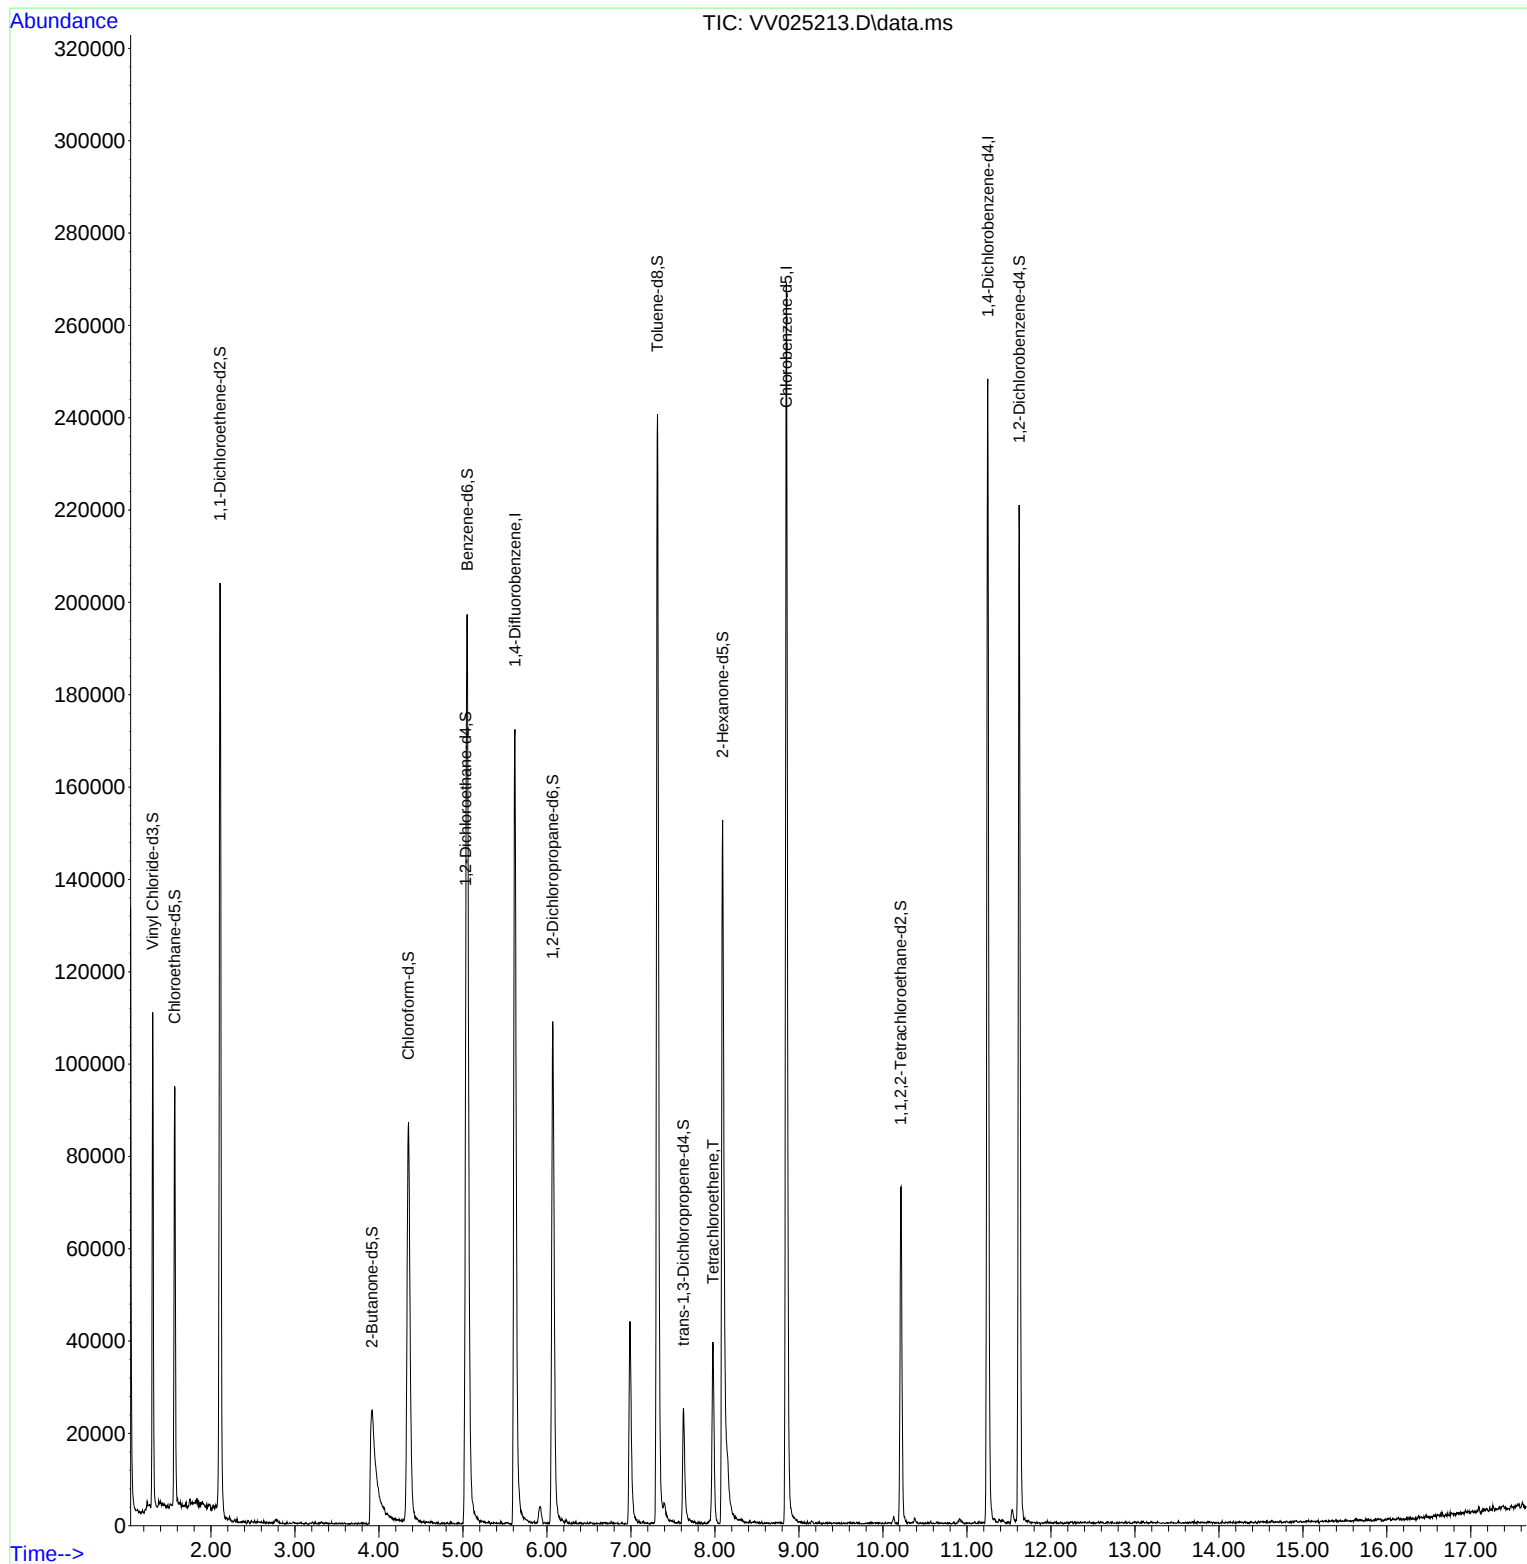

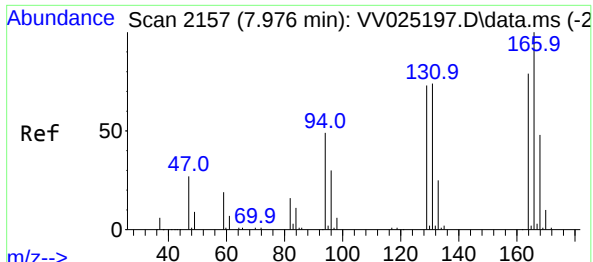

#47
Tetrachloroethene
Concen: 0.919 ug/L
RT: 7.979 min Scan# 21
Delta R.T. 0.003 min
Lab File: VV025213.D
Acq: 26 Mar 2022 21:07

Instrument :
MSVOA_V
ClientSampleId :
C0AD6

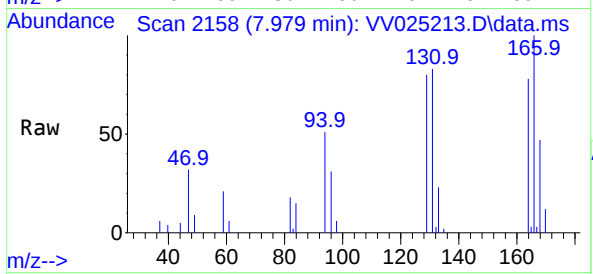

Tgt Ion:164 Resp: 8287

Ion	Ratio	Lower	Upper
164	100		
129	101.5	67.5	125.4
131	105.3	68.0	126.4
166	127.6	86.2	160.2

