

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032622\
 Data File : VW025234.D
 Acq On : 27 Mar 2022 05:41
 Operator : SY/MD
 Sample : N2110-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0PB6

Manual Integrations
 APPROVED

Reviewed By : John Carlone 03/28/2022
 Supervised By : Mahesh Dadoda 03/28/2022

Quant Time: Mar 28 03:49:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Mar 28 03:13:34 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	145602	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	136650	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	59020	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	60868	4.475	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	89.600%	
7) Chloroethane-d5	1.571	69	55264	4.841	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	96.800%	
11) 1,1-Dichloroethene-d2	2.111	63	99524	3.378	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	67.600%	
20) 2-Butanone-d5	3.912	46	63379	46.782	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	93.560%	
24) Chloroform-d	4.349	84	89615	5.049	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.000%	
26) 1,2-Dichloroethane-d4	5.037	65	41293	5.263	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	105.200%	
32) Benzene-d6	5.053	84	180983	5.235	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	104.800%	
36) 1,2-Dichloropropane-d6	6.072	67	52099	5.377	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	107.600%	
41) Toluene-d8	7.317	98	156223	4.927	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	98.600%	
43) trans-1,3-Dichloroprop...	7.625	79	14916	4.719	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	94.400%	
46) 2-Hexanone-d5	8.088	63	66639	58.377	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	116.760%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	32035	4.959	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	99.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	52880	5.579	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	111.600%	
Target Compounds						
12) 1,1-Dichloroethene	2.114	96	1943	0.133	ug/L #	1
17) Methyl tert-butyl Ether	2.774	73	11463	0.618	ug/L #	90
18) trans-1,2-Dichloroethene	2.767	96	648	0.062	ug/L	81
22) cis-1,2-Dichloroethene	3.915	96	25417	2.378	ug/L	100
25) Chloroform	4.378	83	9044	0.464	ug/L	95
34) Trichloroethene	5.918	95	34372	3.123	ug/L	98
47) Tetrachloroethene	7.982	164	21429288m	2640.408	ug/L	
51) Chlorobenzene	8.883	112	2439	0.088	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Reviewed By :John Carlone 03/28/2022
Supervised By :Mahesh Dadoda 03/28/2022

Page: 2

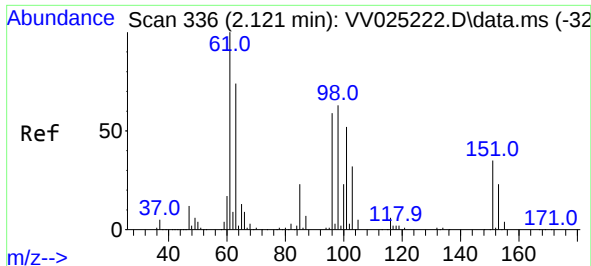

#12
1,1-Dichloroethene
Concen: 0.133 ug/L
RT: 2.114 min Scan# 311
Delta R.T. -0.006 min
Lab File: VV025234.D
Acq: 27 Mar 2022 05:41




Instrument :
MSVOA_V
ClientSampleId :
C0PB6

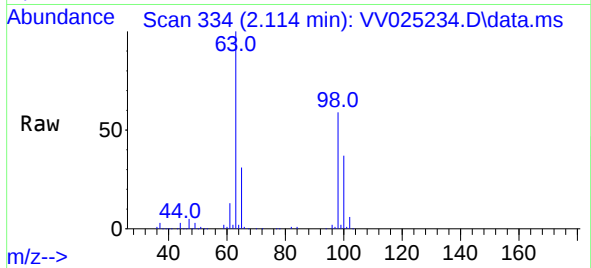

Tgt Ion: 96 Resp: 194
Ion Ratio Lower Upper
96 100
61 683.2 121.5 225.7
63 5084.9 77.9 144.7




Manual Integrations
APPROVED


Reviewed By :John Carlone 03/28/2022
Supervised By :Mahesh Dadoda 03/28/2022

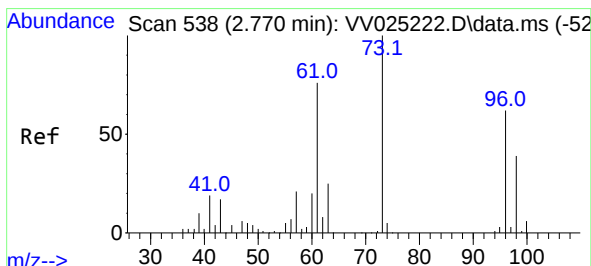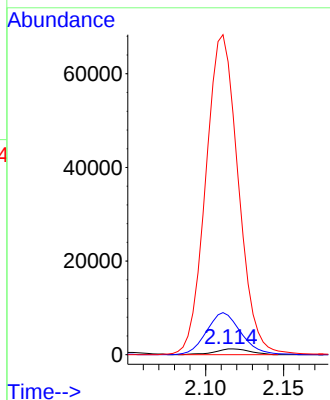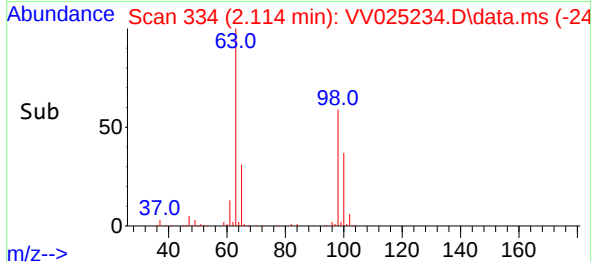

#17
Methyl tert-butyl Ether
Concen: 0.618 ug/L
RT: 2.774 min Scan# 539
Delta R.T. 0.003 min
Lab File: VV025234.D
Acq: 27 Mar 2022 05:41


Tgt Ion: 73 Resp: 11463
Ion Ratio Lower Upper
73 100
43 22.5 13.5 20.3
57 23.9 16.4 24.6

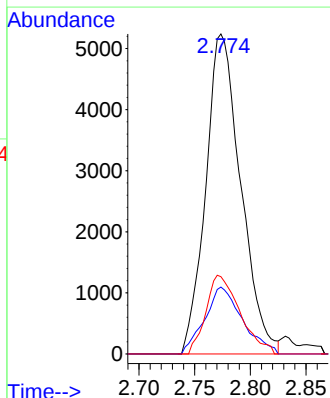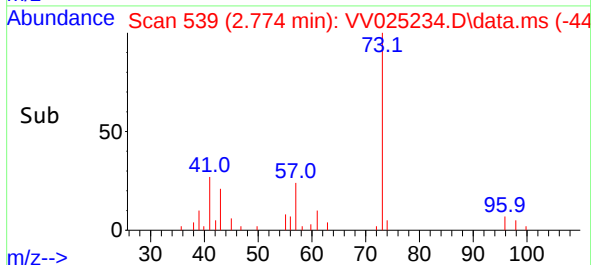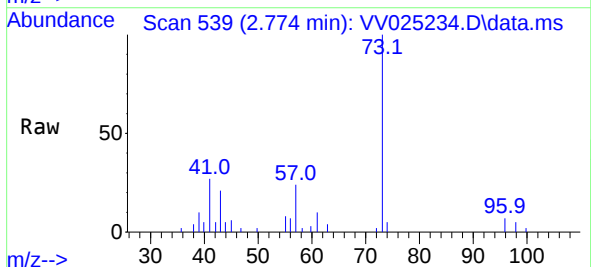

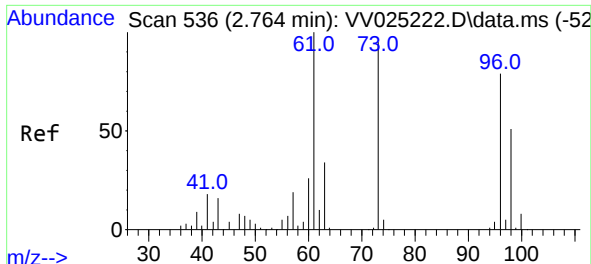

#18
trans-1,2-Dichloroethene
Concen: 0.062 ug/L
RT: 2.767 min Scan# 51
Delta R.T. 0.003 min
Lab File: VV025234.D
Acq: 27 Mar 2022 05:41




Instrument :
MSVOA_V
ClientSampleId :
C0PB6

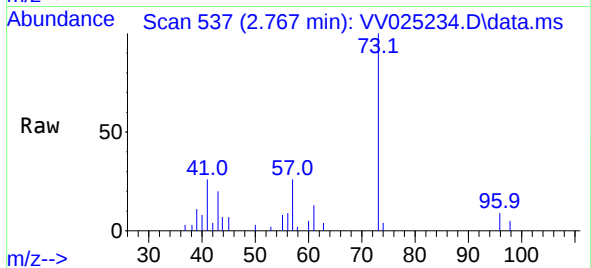


Tgt Ion: 96 Resp: 648
Ion Ratio Lower Upper
96 100
61 156.5 87.6 162.8
98 62.3 44.0 81.8

Manual Integrations
APPROVED



Reviewed By :John Carlone 03/28/2022
Supervised By :Mahesh Dadoda 03/28/2022

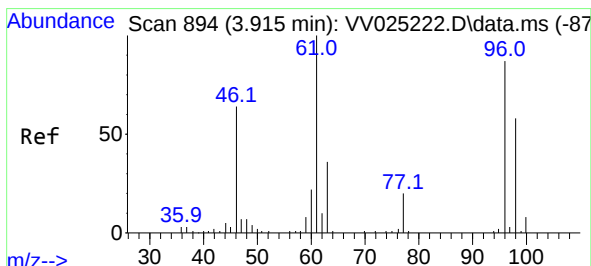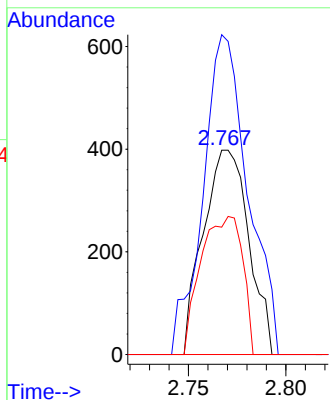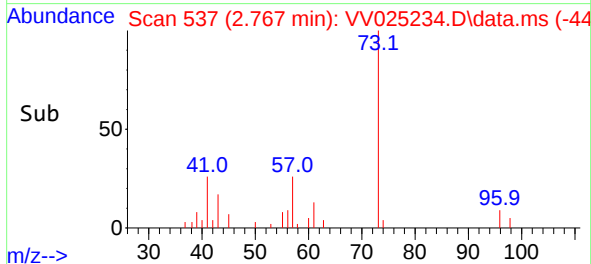


#22
cis-1,2-Dichloroethene
Concen: 2.378 ug/L
RT: 3.915 min Scan# 894
Delta R.T. 0.000 min
Lab File: VV025234.D
Acq: 27 Mar 2022 05:41

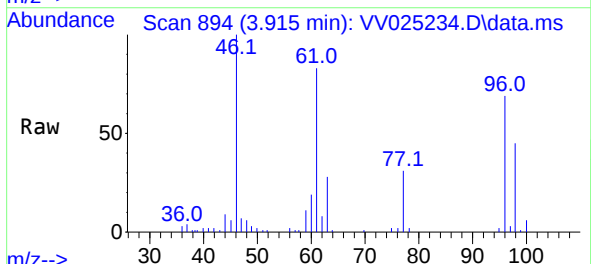

Tgt Ion: 96 Resp: 25417
Ion Ratio Lower Upper
96 100
61 120.5 84.1 156.1
68 0.0 0.0 0.0

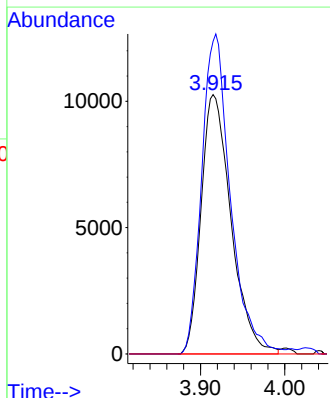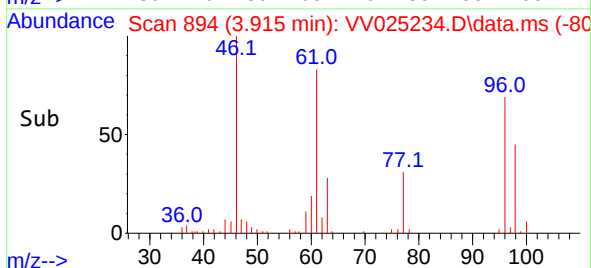

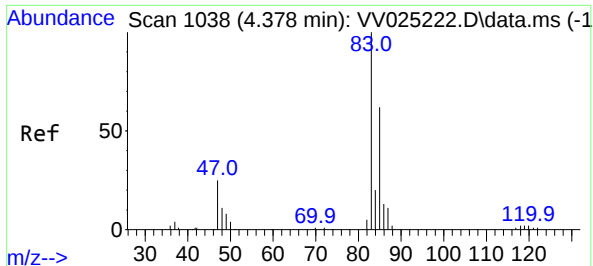

#25

Chloroform

Concen: 0.464 ug/L

RT: 4.378 min Scan# 1038

Delta R.T. 0.000 min

Lab File: VV025234.D

Acq: 27 Mar 2022 05:41

Instrument :

MSVOA_V

ClientSampleId :





C0PB6

Tgt Ion: 83 Resp: 9044
 Ion Ratio Lower Upper
 83 100
 85 59.8 44.7 82.9

Manual Integrations

APPROVED

Reviewed By :John Carlone 03/28/2022
 Supervised By :Mahesh Dadoda 03/28/2022

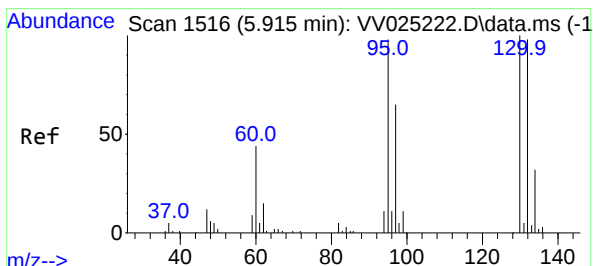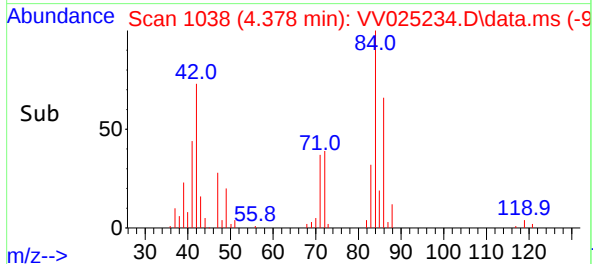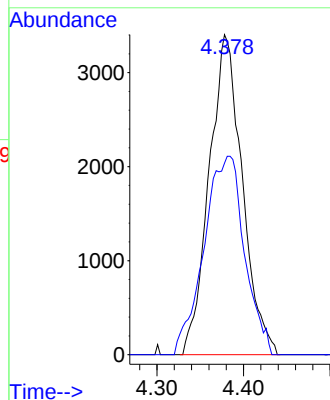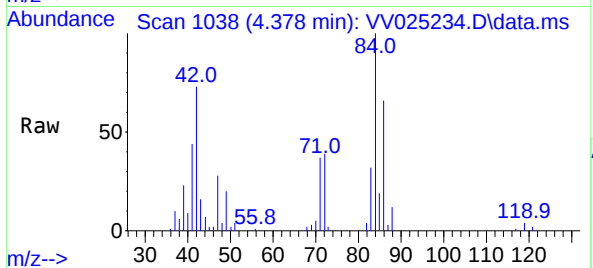

#34

Trichloroethene

Concen: 3.123 ug/L




RT: 5.918 min Scan# 1517


Delta R.T. 0.003 min

Lab File: VV025234.D

Acq: 27 Mar 2022 05:41


Tgt Ion: 95 Resp: 34372
 Ion Ratio Lower Upper
 95 100
 97 64.8 46.3 85.9
 132 93.0 65.2 121.2
 130 98.6 71.7 133.1

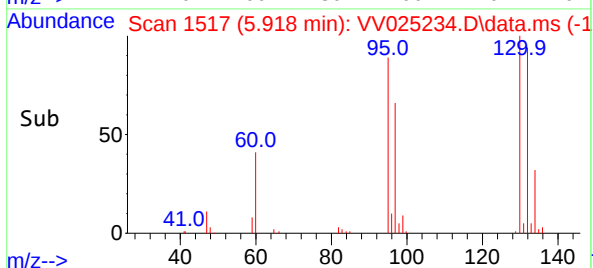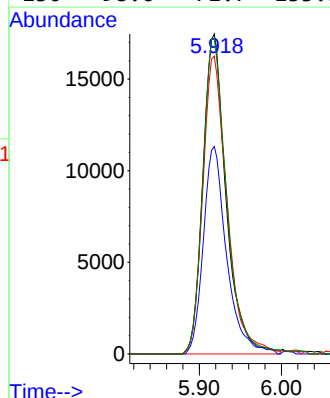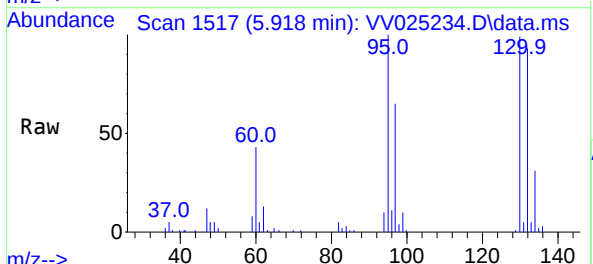

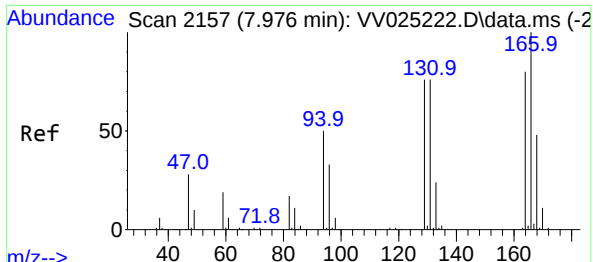

#47
Tetrachloroethene
Concen: 2640.408 ug/L m
RT: 7.982 min Scan# 2157
Delta R.T. 0.007 min
Lab File: VV025234.D
Acq: 27 Mar 2022 05:41




Instrument :
MSVOA_V
ClientSampleId :
C0PB6

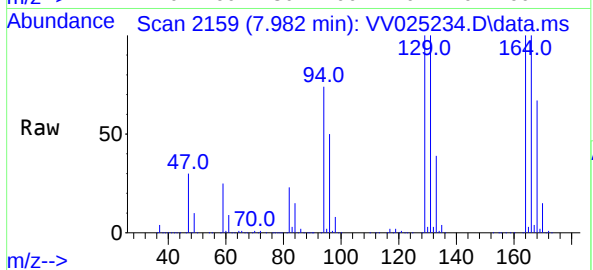


Tgt Ion:164 Resp:2142928
Ion Ratio Lower Upper
164 100
129 100.0 67.5 125.4
131 100.0 68.0 126.4
166 100.0 86.2 160.2

Manual Integrations
APPROVED

Reviewed By :John Carlone 03/28/2022
Supervised By :Mahesh Dadoda 03/28/2022

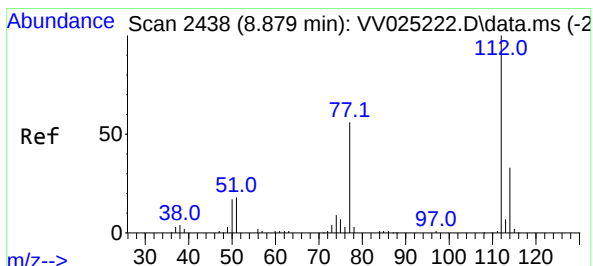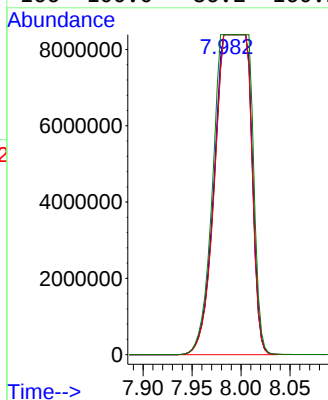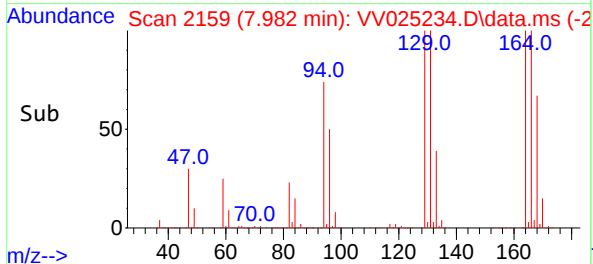

#51
Chlorobenzene
Concen: 0.088 ug/L
RT: 8.883 min Scan# 2439
Delta R.T. 0.003 min
Lab File: VV025234.D
Acq: 27 Mar 2022 05:41

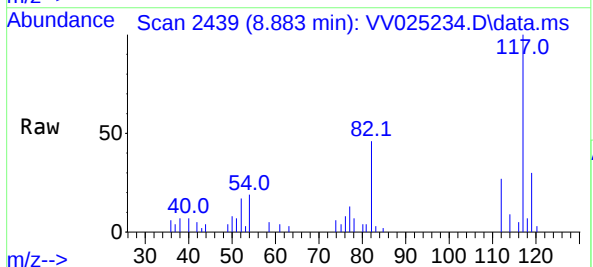

Tgt Ion:112 Resp: 2439
Ion Ratio Lower Upper
112 100
114 34.2 21.9 40.7
77 48.1 44.2 66.4

