

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
 Data File : VV025200.D
 Acq On : 26 Mar 2022 16:02
 Operator : SY/MD
 Sample : N2083-04DL 10X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW5Z7DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025200.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	95	rVB	113162	116731	24.08%	2.792%
2	1.568	157	164	173	rBV	98366	110037	22.69%	2.632%
3	2.108	320	332	359	rVB	210709	321351	66.28%	7.687%
4	2.510	449	457	466	rBV5	5107	8203	1.69%	0.196%
5	3.191	653	669	685	rBV2	10928	23681	4.88%	0.566%
6	3.918	884	895	898	rBV3	25884	42980	8.86%	1.028%
7	4.352	1013	1030	1059	rBV	82198	214351	44.21%	5.128%
8	4.609	1093	1110	1132	rBV2	54572	136921	28.24%	3.275%
9	5.046	1228	1246	1272	rBV2	198152	484852	100.00%	11.598%
10	5.619	1409	1424	1453	rBV	167238	346818	71.53%	8.296%
11	5.921	1506	1518	1534	rBV10	6074	14549	3.00%	0.348%
12	6.069	1552	1564	1586	rBV	107384	225772	46.57%	5.401%
13	6.989	1839	1850	1876	rBV2	44425	88138	18.18%	2.108%
14	7.316	1939	1952	1972	rBV	237181	417296	86.07%	9.982%
15	7.625	2039	2048	2067	rBV	25948	47875	9.87%	1.145%
16	8.091	2182	2193	2228	rBV	153522	334266	68.94%	7.996%
17	8.850	2415	2429	2448	rBV	250550	417466	86.10%	9.986%
18	10.217	2837	2854	2869	rBV	71339	113100	23.33%	2.706%
19	11.249	3162	3175	3196	rBV	235969	377841	77.93%	9.039%
20	11.622	3280	3291	3308	rBV	213198	338085	69.73%	8.088%




Sum of corrected areas: 4180313

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025200.D
Acq On : 26 Mar 2022 16:02
Operator : SY/MD
Sample : N2083-04DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW5Z7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

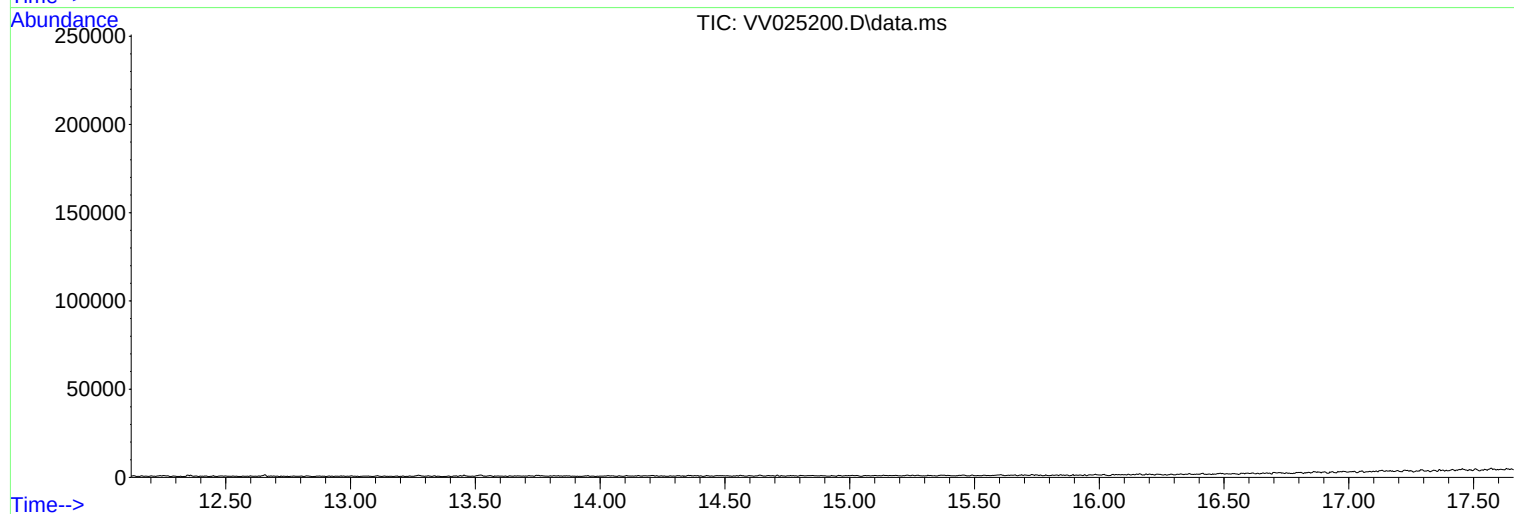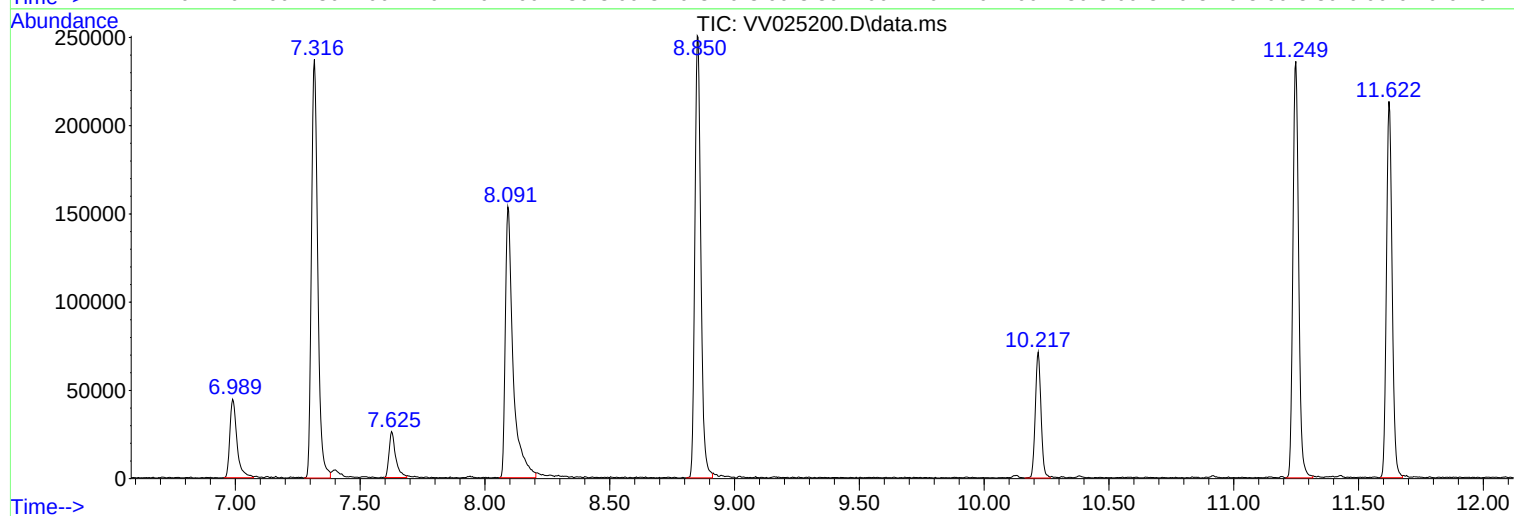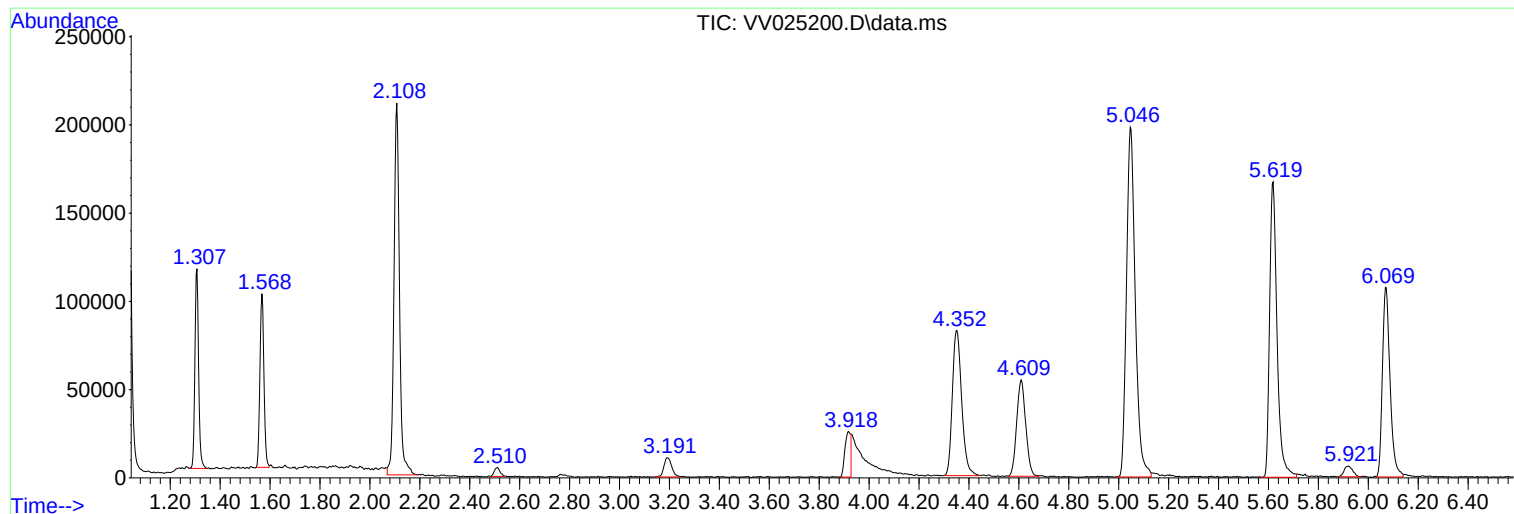

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025200.D
Acq On : 26 Mar 2022 16:02
Operator : SY/MD
Sample : N2083-04DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW5Z7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025200.D
Acq On : 26 Mar 2022 16:02
Operator : SY/MD
Sample : N2083-04DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW5Z7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
