

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
 Data File : VV025203.D
 Acq On : 26 Mar 2022 17:12
 Operator : SY/MD
 Sample : N2083-15
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025203.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	50	62	65	rBV7	3013	5237	1.03%	0.125%
2	1.307	74	83	94	rBV	120538	120151	23.67%	2.875%
3	1.568	156	164	180	rVB	100848	113862	22.43%	2.724%
4	2.108	317	332	354	rVB	218542	329713	64.96%	7.888%
5	2.513	448	458	468	rBV5	5787	10160	2.00%	0.243%
6	3.918	882	895	919	rBV2	23584	100732	19.84%	2.410%
7	4.352	1014	1030	1056	rBV	87807	219657	43.27%	5.255%
8	5.050	1230	1247	1275	rBV2	202579	507601	100.00%	12.145%
9	5.619	1412	1424	1447	rBV	166749	342998	67.57%	8.206%
10	5.915	1504	1516	1529	rVB8	4273	8620	1.70%	0.206%
11	6.072	1552	1565	1588	rBV	113808	234502	46.20%	5.611%
12	6.989	1839	1850	1868	rBV	46337	90709	17.87%	2.170%
13	7.317	1938	1952	1971	rBV	246739	437110	86.11%	10.458%
14	7.625	2038	2048	2068	rBV	27074	50864	10.02%	1.217%
15	8.091	2183	2193	2230	rBV2	153349	338567	66.70%	8.100%
16	8.850	2419	2429	2453	rBV	260174	426269	83.98%	10.199%
17	10.217	2843	2854	2871	rBV	72860	113747	22.41%	2.721%
18	11.249	3164	3175	3202	rBV	243975	378963	74.66%	9.067%
19	11.622	3279	3291	3307	rBV	223235	350210	68.99%	8.379%




Sum of corrected areas: 4179672

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025203.D
Acq On : 26 Mar 2022 17:12
Operator : SY/MD
Sample : N2083-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

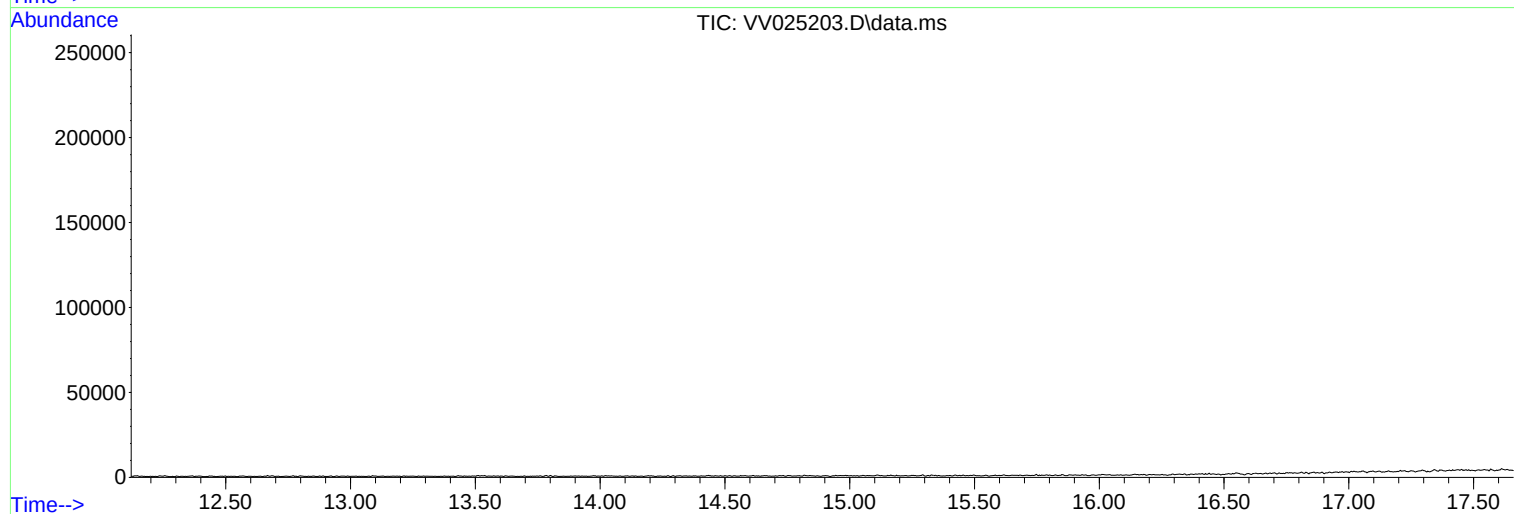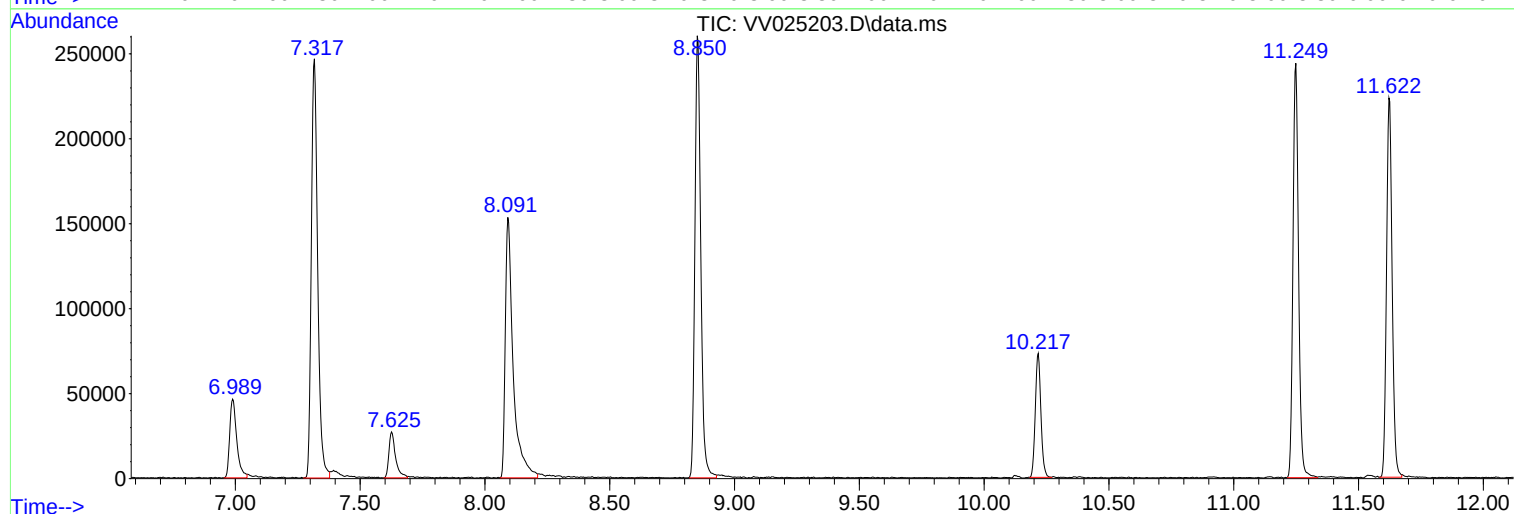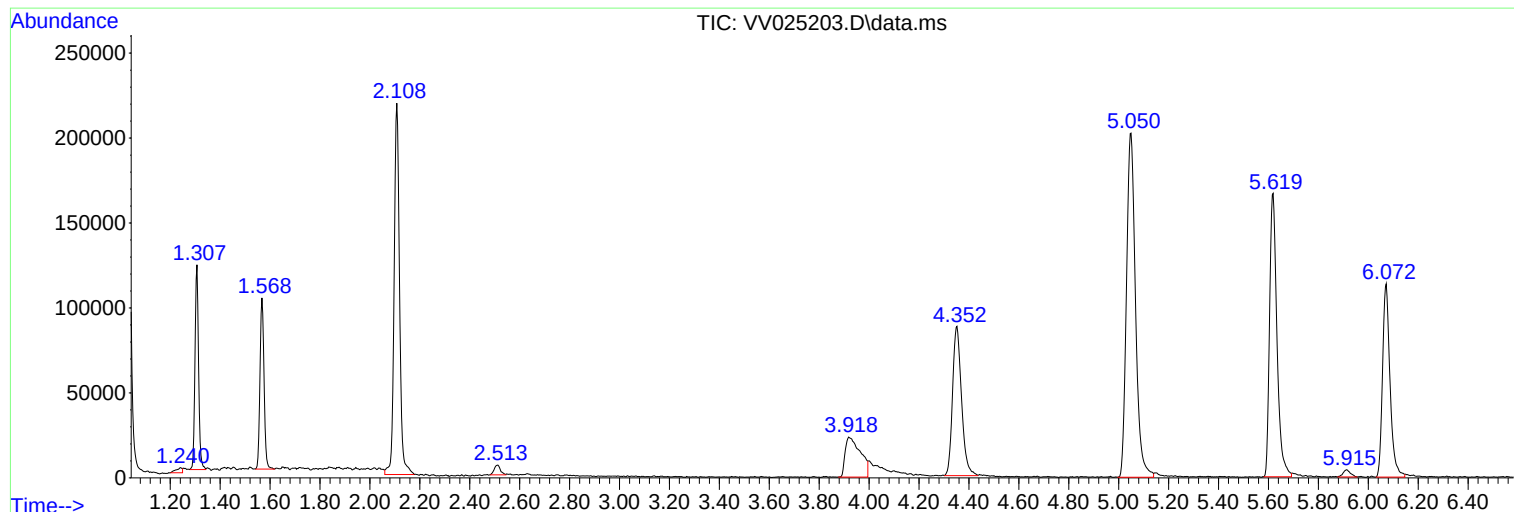

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025203.D
Acq On : 26 Mar 2022 17:12
Operator : SY/MD
Sample : N2083-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025203.D
Acq On : 26 Mar 2022 17:12
Operator : SY/MD
Sample : N2083-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------