

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
 Data File : VV025204.D
 Acq On : 26 Mar 2022 17:36
 Operator : SY/MD
 Sample : N2082-15
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW612

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025204.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	47	55	68	rBV	165691	150349	30.65%	3.559%
2	1.307	74	83	94	rBV	106241	115946	23.64%	2.745%
3	1.571	156	165	174	rBV	94572	106275	21.67%	2.516%
4	2.111	322	333	353	rVB	191297	282064	57.51%	6.677%
5	3.899	877	889	914	rBV	36202	118611	24.18%	2.808%
6	4.349	1013	1029	1056	rBV	88744	229703	46.83%	5.438%
7	5.047	1225	1246	1271	rBV2	195936	490502	100.00%	11.611%
8	5.619	1412	1424	1453	rBV	163024	340610	69.44%	8.063%
9	5.912	1506	1515	1524	rBV6	4318	8531	1.74%	0.202%
10	6.072	1552	1565	1583	rBV	108925	227152	46.31%	5.377%
11	6.989	1839	1850	1872	rBV	46292	89371	18.22%	2.116%
12	7.317	1939	1952	1969	rBV	238838	424983	86.64%	10.060%
13	7.394	1970	1976	1995	rVB2	10589	22609	4.61%	0.535%
14	7.625	2039	2048	2065	rBV	24956	47182	9.62%	1.117%
15	8.088	2181	2192	2226	rBV	162107	322985	65.85%	7.646%
16	8.850	2418	2429	2447	rBV	254786	418061	85.23%	9.896%
17	10.214	2843	2853	2867	rBV2	67940	108088	22.04%	2.559%
18	11.249	3163	3175	3201	rBV	241641	374164	76.28%	8.857%
19	11.622	3280	3291	3309	rBV	216846	341310	69.58%	8.080%
20	12.349	3509	3517	3528	rBV7	3710	5850	1.19%	0.138%




Sum of corrected areas: 4224346

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025204.D
Acq On : 26 Mar 2022 17:36
Operator : SY/MD
Sample : N2082-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW612

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

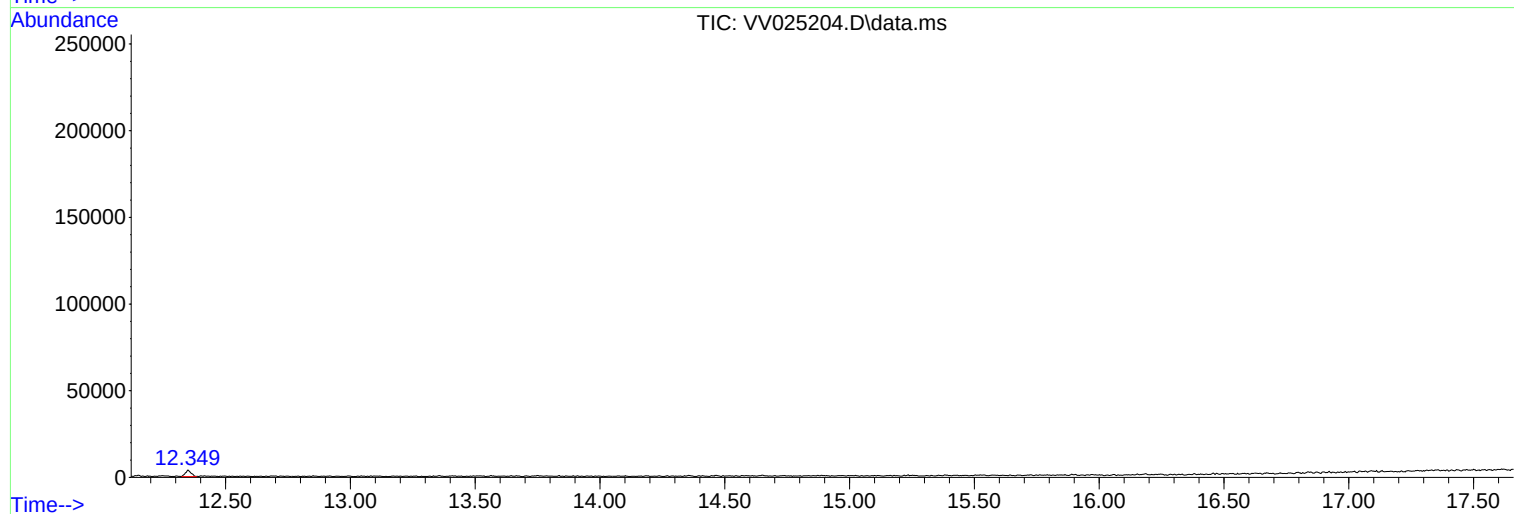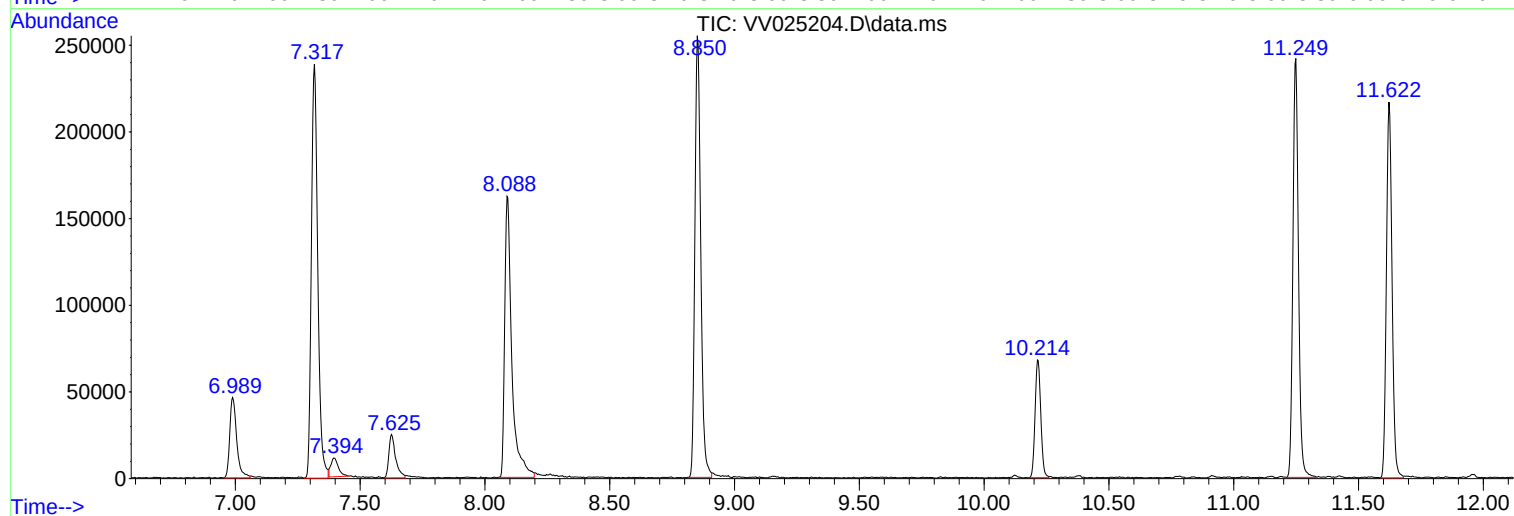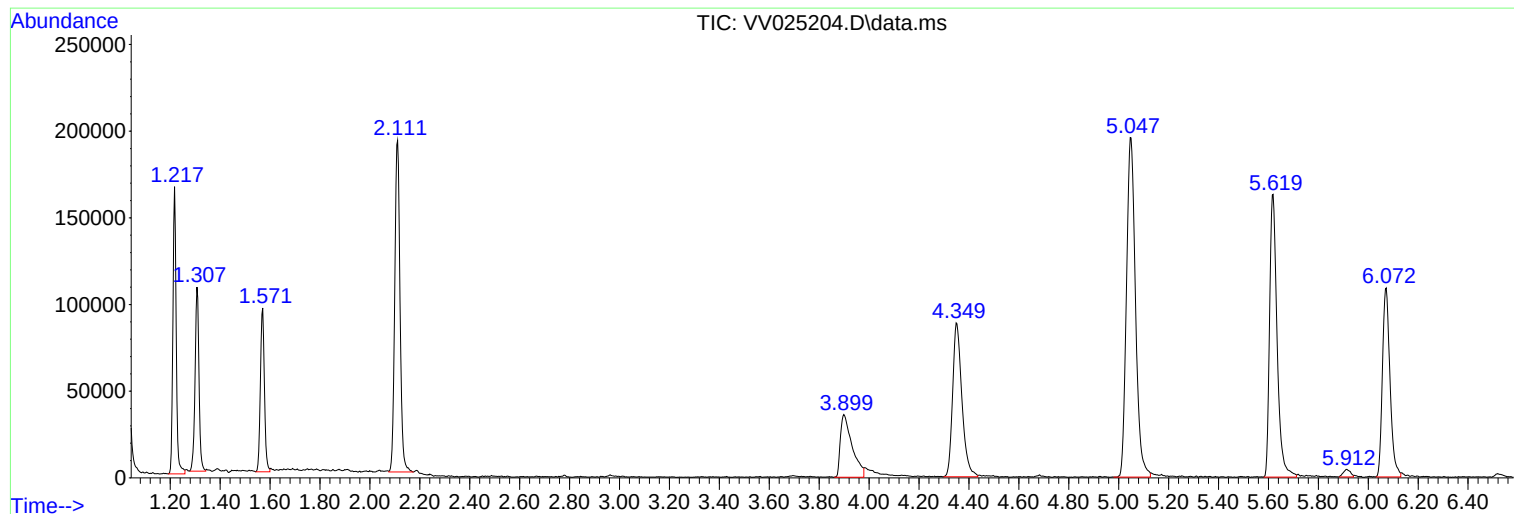

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025204.D
Acq On : 26 Mar 2022 17:36
Operator : SY/MD
Sample : N2082-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW612










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.217	2.21 ug/L	150349	1,4-Difluorobenzene	5.619

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Isobutane	58	C4H10	000075-28-5	64
2		Isobutane	58	C4H10	000075-28-5	64
3		Isobutane	58	C4H10	000075-28-5	64
4		Isobutane	58	C4H10	000075-28-5	64
5		Isobutane	58	C4H10	000075-28-5	45

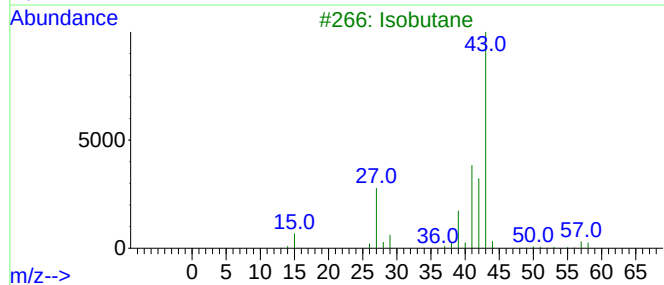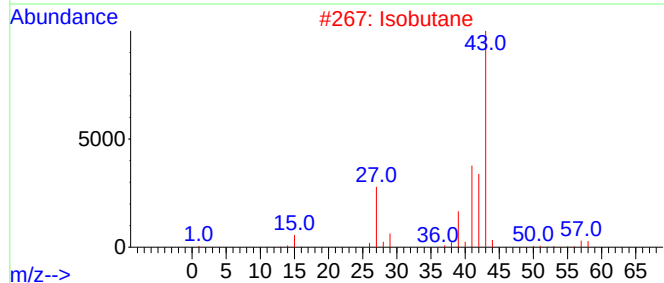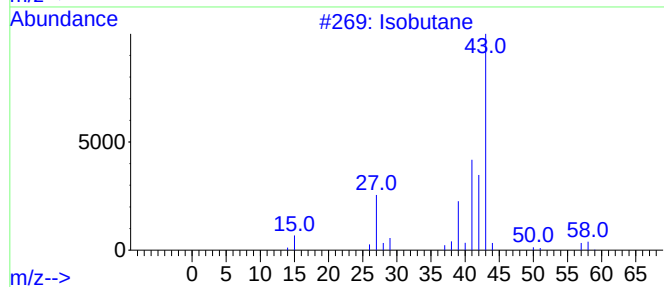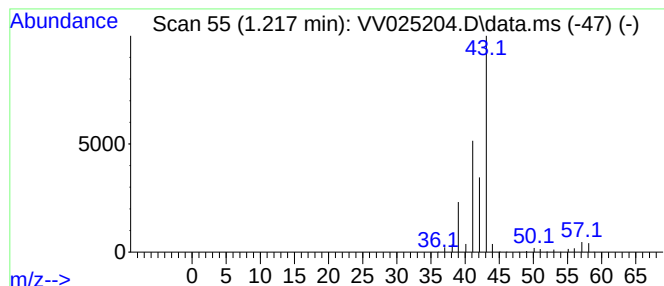

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032622\
Data File : VW025204.D
Acq On : 26 Mar 2022 17:36
Operator : SY/MD
Sample : N2082-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW612

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	1.217	2.2	ug/L	150349	1	5.619	340610	5.0