

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
 Data File : VV025205.D
 Acq On : 26 Mar 2022 17:59
 Operator : SY/MD
 Sample : N2082-16
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW615

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025205.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	48	55	65	rBV	167916	150725	29.60%	3.439%
2	1.307	74	83	94	rBV	109494	118621	23.30%	2.706%
3	1.568	157	164	178	rBV	94541	110691	21.74%	2.525%
4	2.111	320	333	352	rVB	196854	291855	57.32%	6.659%
5	3.902	879	890	923	rBV2	34775	125505	24.65%	2.863%
6	4.352	1014	1030	1056	rBV2	90126	236944	46.54%	5.406%
7	5.047	1231	1246	1274	rBV3	204784	509149	100.00%	11.617%
8	5.616	1412	1423	1452	rBV	172479	358520	70.42%	8.180%
9	5.915	1504	1516	1529	rBV9	5430	11429	2.24%	0.261%
10	6.069	1551	1564	1587	rBV2	112447	236665	46.48%	5.400%
11	6.989	1839	1850	1873	rBV	47615	89775	17.63%	2.048%
12	7.317	1940	1952	1968	rBV	251079	439905	86.40%	10.037%
13	7.397	1969	1977	1993	rVB	12546	25326	4.97%	0.578%
14	7.625	2040	2048	2062	rBV	26114	45992	9.03%	1.049%
15	8.088	2181	2192	2224	rBV	162788	328880	64.59%	7.504%
16	8.850	2417	2429	2448	rBV	269208	442770	86.96%	10.102%
17	10.214	2842	2853	2868	rBV	71034	112358	22.07%	2.564%
18	11.249	3163	3175	3194	rBV	247790	388512	76.31%	8.864%
19	11.622	3280	3291	3306	rBV	226157	354245	69.58%	8.082%
20	12.349	3508	3517	3525	rBV8	3347	5096	1.00%	0.116%




Sum of corrected areas: 4382963

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025205.D
Acq On : 26 Mar 2022 17:59
Operator : SY/MD
Sample : N2082-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW615

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

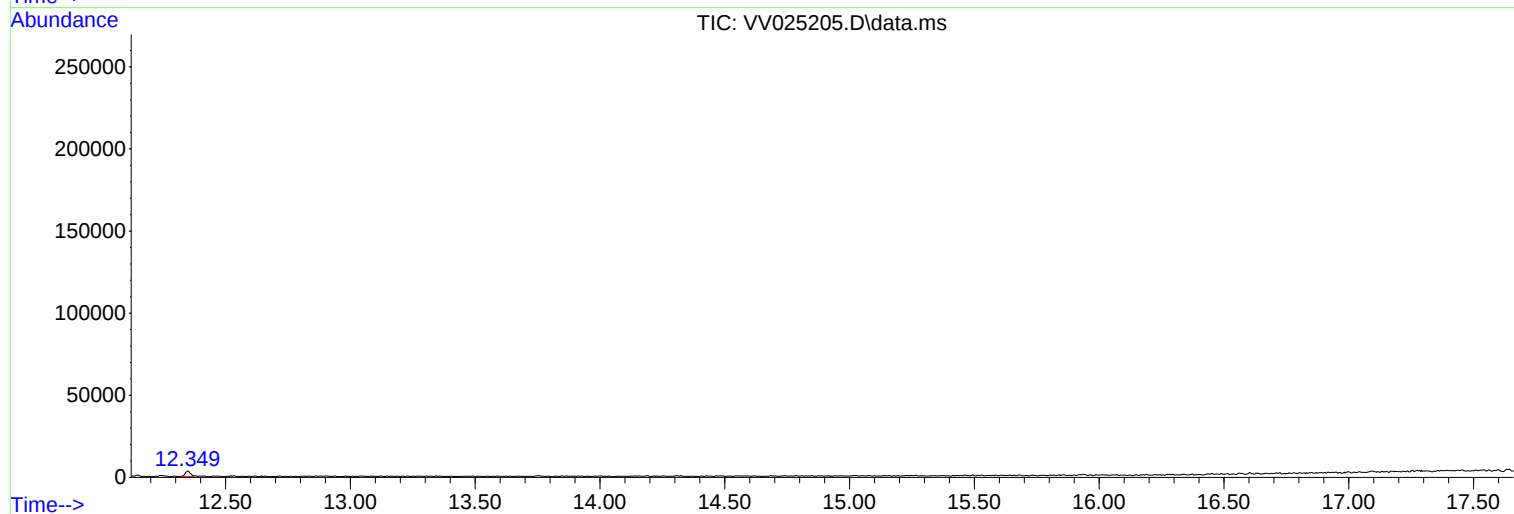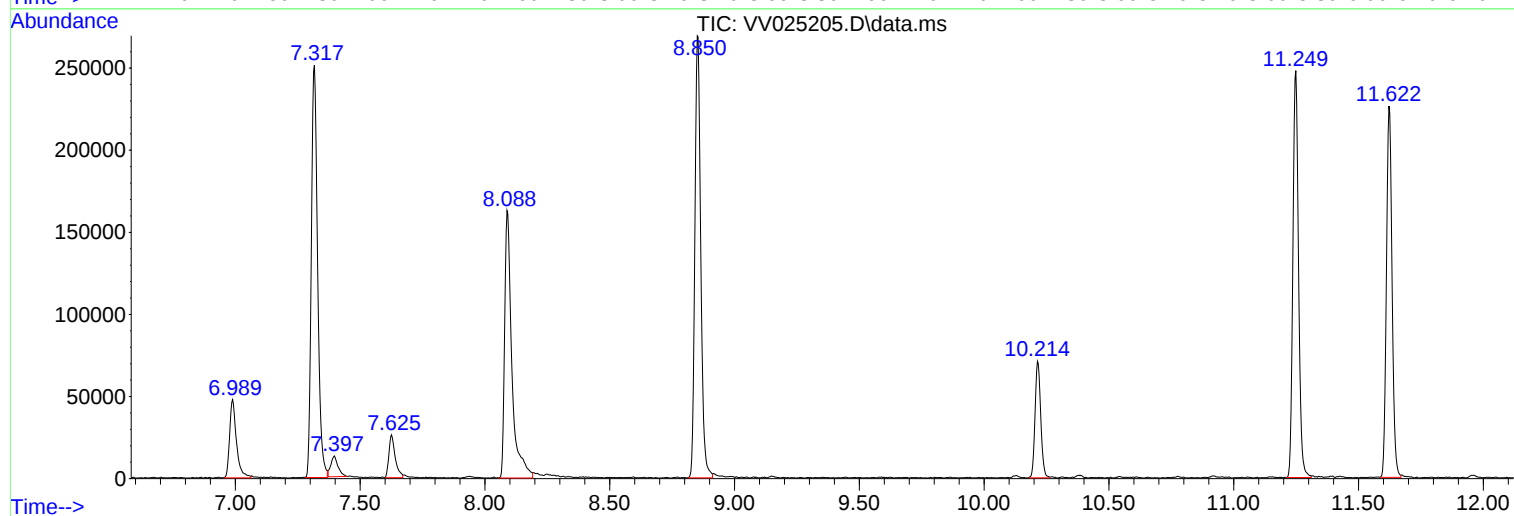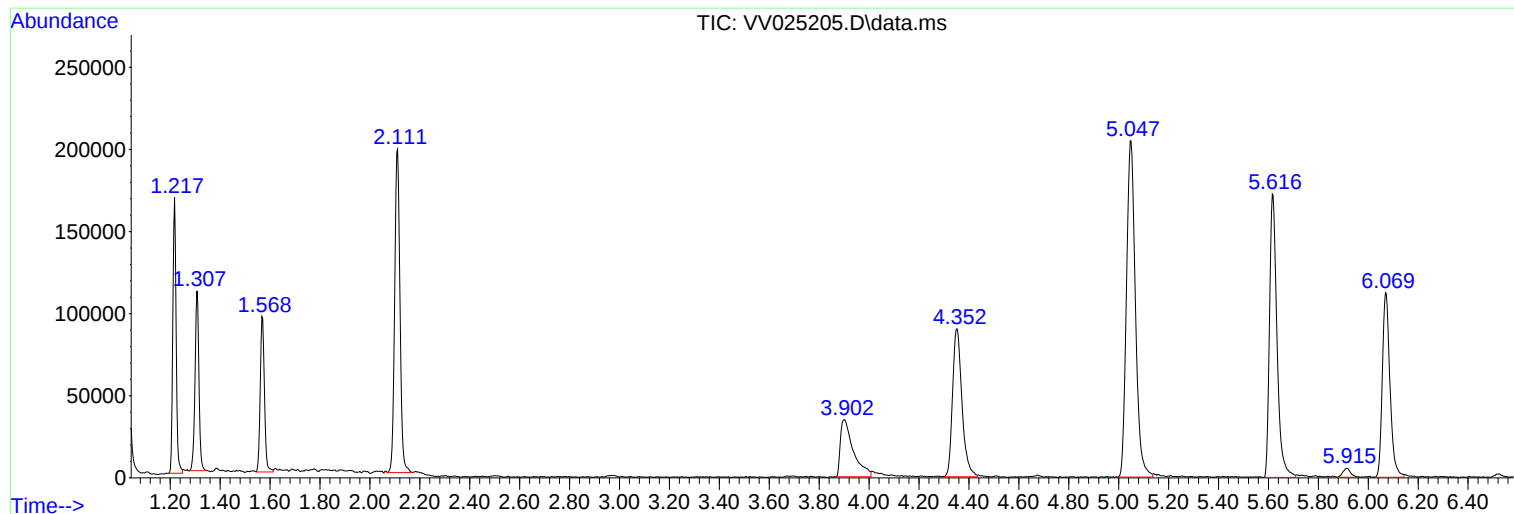

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025205.D
Acq On : 26 Mar 2022 17:59
Operator : SY/MD
Sample : N2082-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW615










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.217	2.10 ug/L	150725	1,4-Difluorobenzene	5.616

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Isobutane	58	C4H10	000075-28-5	72
2		Isobutane	58	C4H10	000075-28-5	64
3		Isobutane	58	C4H10	000075-28-5	64
4		Isobutane	58	C4H10	000075-28-5	64
5		Isobutane	58	C4H10	000075-28-5	45

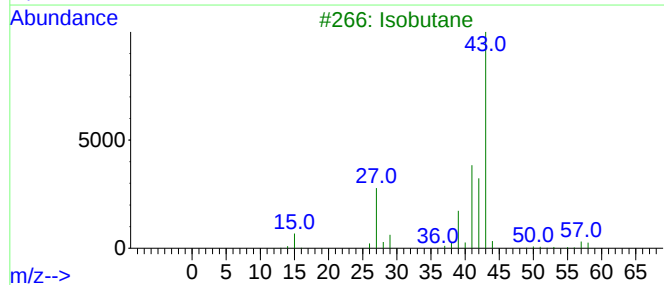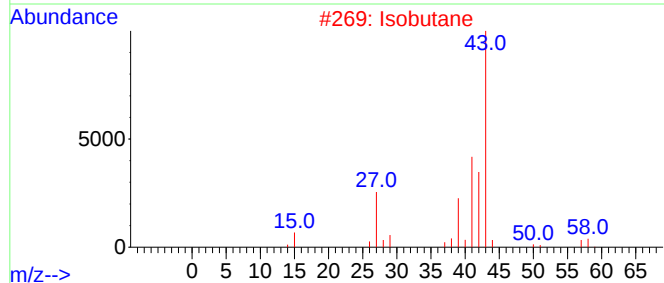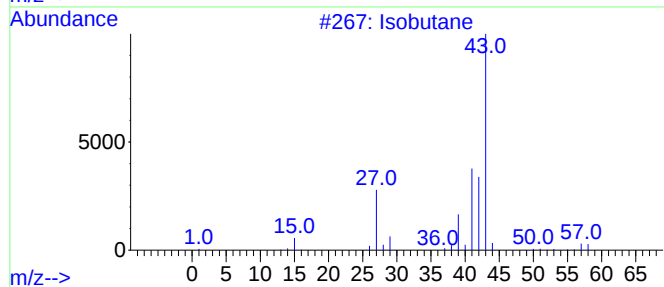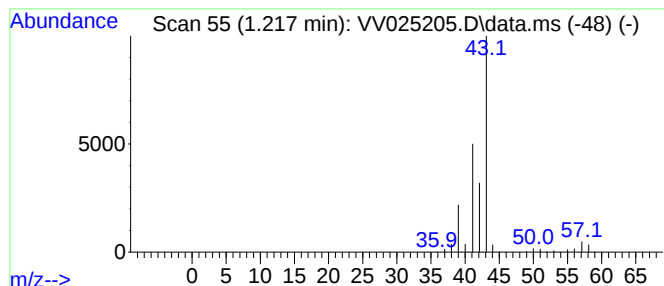

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032622\
Data File : VW025205.D
Acq On : 26 Mar 2022 17:59
Operator : SY/MD
Sample : N2082-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW615

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	1.217	2.1	ug/L	150725	1	5.616	358520	5.0