

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
 Data File : VV025208.D
 Acq On : 26 Mar 2022 19:09
 Operator : SY/MD
 Sample : N2097-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025208.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB	101869	104124	21.10%	2.388%
2	1.571	156	165	175	rBV	91740	105515	21.38%	2.420%
3	1.757	217	223	231	rVB2	5394	7034	1.43%	0.161%
4	2.111	323	333	352	rVB2	221449	352183	71.38%	8.077%
5	2.770	522	538	560	rBV2	21210	46547	9.43%	1.067%
6	3.195	659	670	687	rBV3	7385	16336	3.31%	0.375%
7	3.905	881	891	921	rBV2	32839	121546	24.63%	2.787%
8	4.352	1014	1030	1062	rBV3	91556	257890	52.27%	5.914%
9	4.609	1092	1110	1129	rBV4	43150	108943	22.08%	2.498%
10	5.050	1229	1247	1271	rBV2	198010	493425	100.00%	11.316%
11	5.619	1412	1424	1448	rBV	168733	351554	71.25%	8.062%
12	5.915	1506	1516	1519	rBV4	4552	6886	1.40%	0.158%
13	6.072	1552	1565	1588	rBV3	108677	230807	46.78%	5.293%
14	6.989	1840	1850	1867	rBV2	45457	85515	17.33%	1.961%
15	7.317	1938	1952	1972	rBV	244244	433252	87.81%	9.936%
16	7.625	2039	2048	2071	rBV2	25345	48189	9.77%	1.105%
17	8.091	2183	2193	2229	rBV2	158411	323332	65.53%	7.415%
18	8.850	2418	2429	2452	rBV	260632	428295	86.80%	9.822%
19	10.214	2843	2853	2866	rBV	71204	112055	22.71%	2.570%
20	11.249	3164	3175	3199	rBV	245876	382747	77.57%	8.777%
21	11.622	3279	3291	3314	rBV	218289	344391	69.80%	7.898%




Sum of corrected areas: 4360566

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025208.D
Acq On : 26 Mar 2022 19:09
Operator : SY/MD
Sample : N2097-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

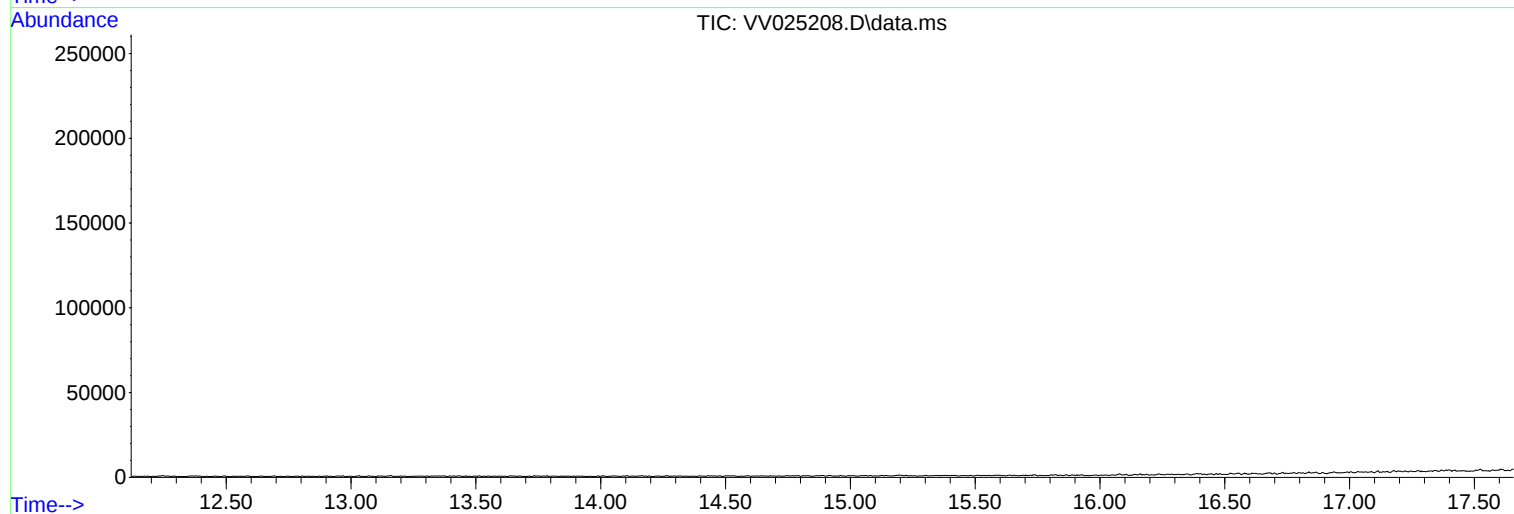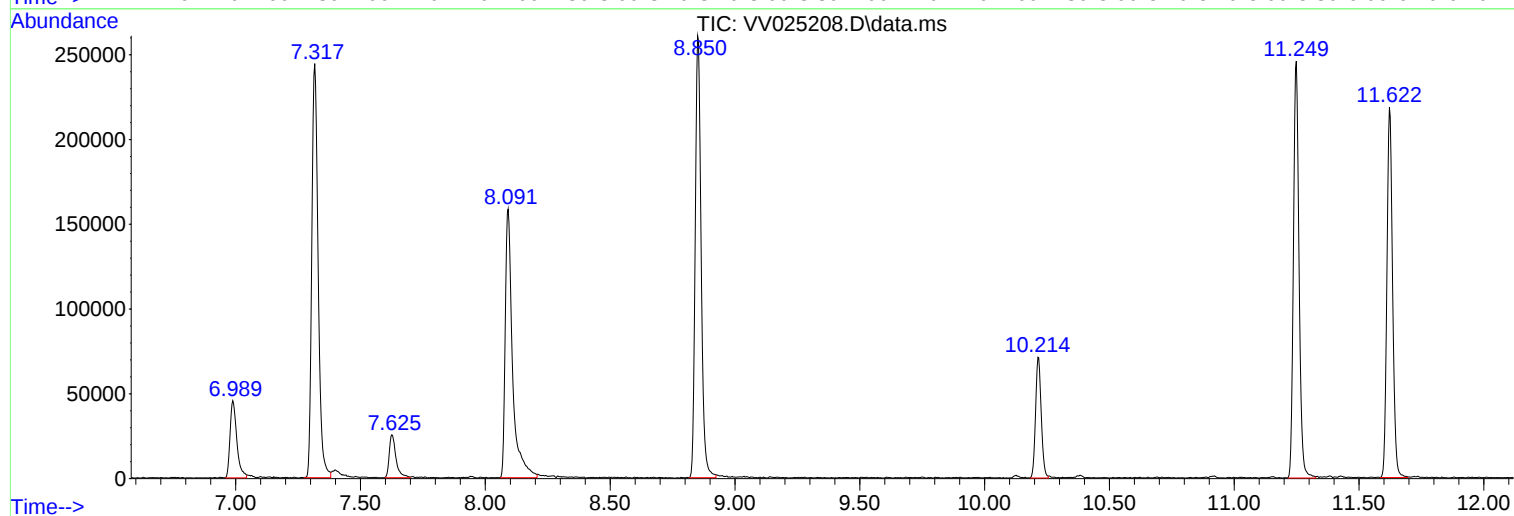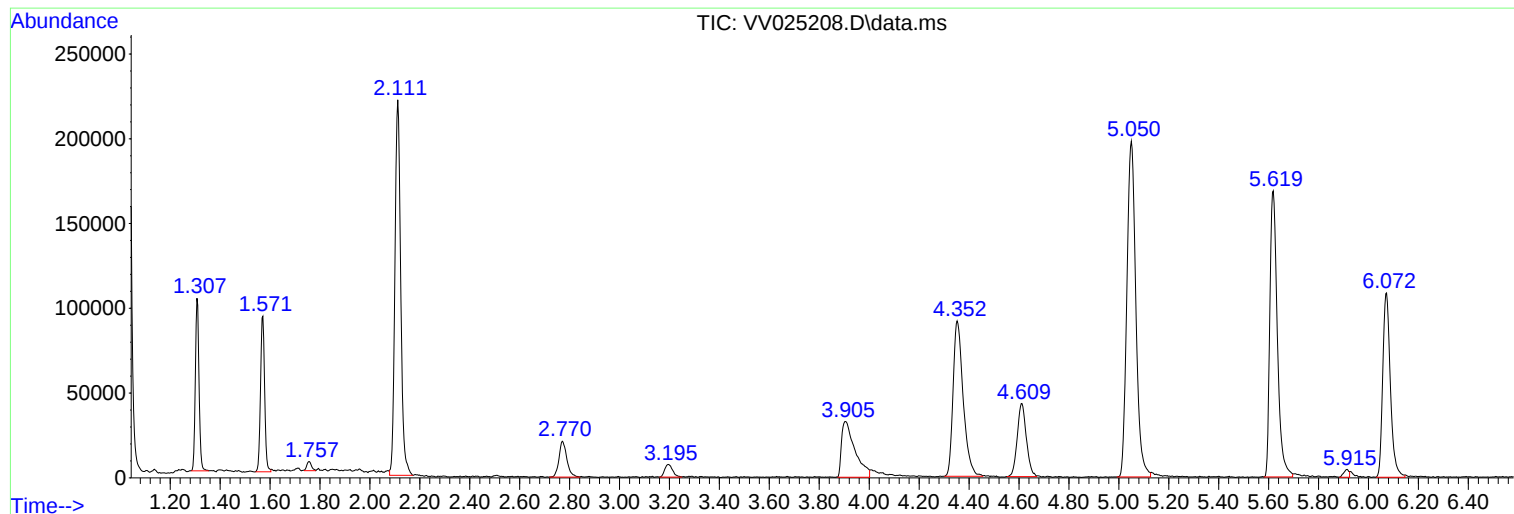

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025208.D
Acq On : 26 Mar 2022 19:09
Operator : SY/MD
Sample : N2097-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025208.D
Acq On : 26 Mar 2022 19:09
Operator : SY/MD
Sample : N2097-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc