

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
 Data File : VV025209.D
 Acq On : 26 Mar 2022 19:33
 Operator : SY/MD
 Sample : N2097-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025209.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	97	rVB	104714	105365	22.29%	2.572%
2	1.568	156	164	174	rBV	88957	100722	21.31%	2.459%
3	1.751	215	221	230	rBV3	3336	4846	1.03%	0.118%
4	2.108	321	332	354	rVB	200927	305560	64.63%	7.458%
5	2.770	522	538	559	rBV3	24322	55524	11.74%	1.355%
6	3.195	656	670	684	rBV	11581	25638	5.42%	0.626%
7	3.912	882	893	917	rBV2	26394	97234	20.57%	2.373%
8	4.352	1014	1030	1062	rBV4	89036	261485	55.31%	6.383%
9	5.047	1229	1246	1277	rBV3	188152	472761	100.00%	11.540%
10	5.619	1411	1424	1449	rBV	171565	349292	73.88%	8.526%
11	5.915	1514	1516	1531	rVB6	3189	5059	1.07%	0.123%
12	6.069	1552	1564	1591	rBV	105169	218773	46.28%	5.340%
13	6.989	1840	1850	1871	rBV	42669	82308	17.41%	2.009%
14	7.317	1940	1952	1971	rBV	228170	405352	85.74%	9.894%
15	7.394	1971	1976	1985	rVB6	2376	4873	1.03%	0.119%
16	7.625	2039	2048	2064	rBV	22506	42282	8.94%	1.032%
17	8.091	2183	2193	2227	rBV	150676	313523	66.32%	7.653%
18	8.850	2418	2429	2450	rBV	256025	428517	90.64%	10.460%
19	10.214	2841	2853	2870	rBV2	65765	107975	22.84%	2.636%
20	11.249	3164	3175	3197	rBV	244390	379717	80.32%	9.269%
21	11.622	3279	3291	3310	rBV	206615	330021	69.81%	8.056%




Sum of corrected areas: 4096827

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025209.D
Acq On : 26 Mar 2022 19:33
Operator : SY/MD
Sample : N2097-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

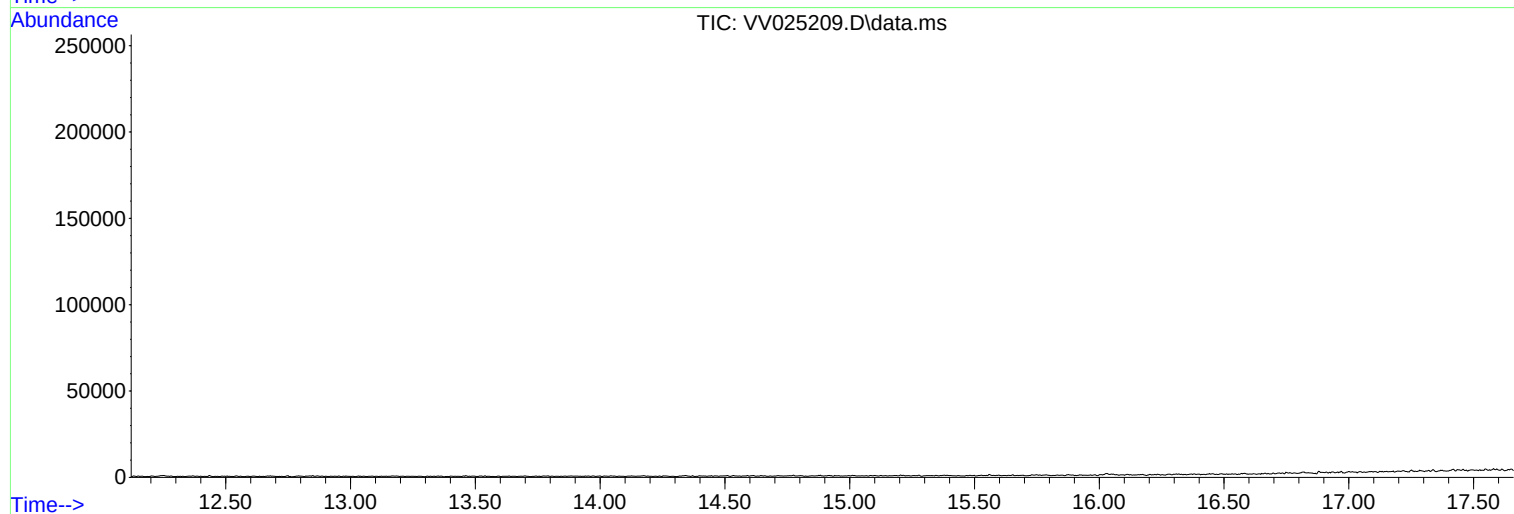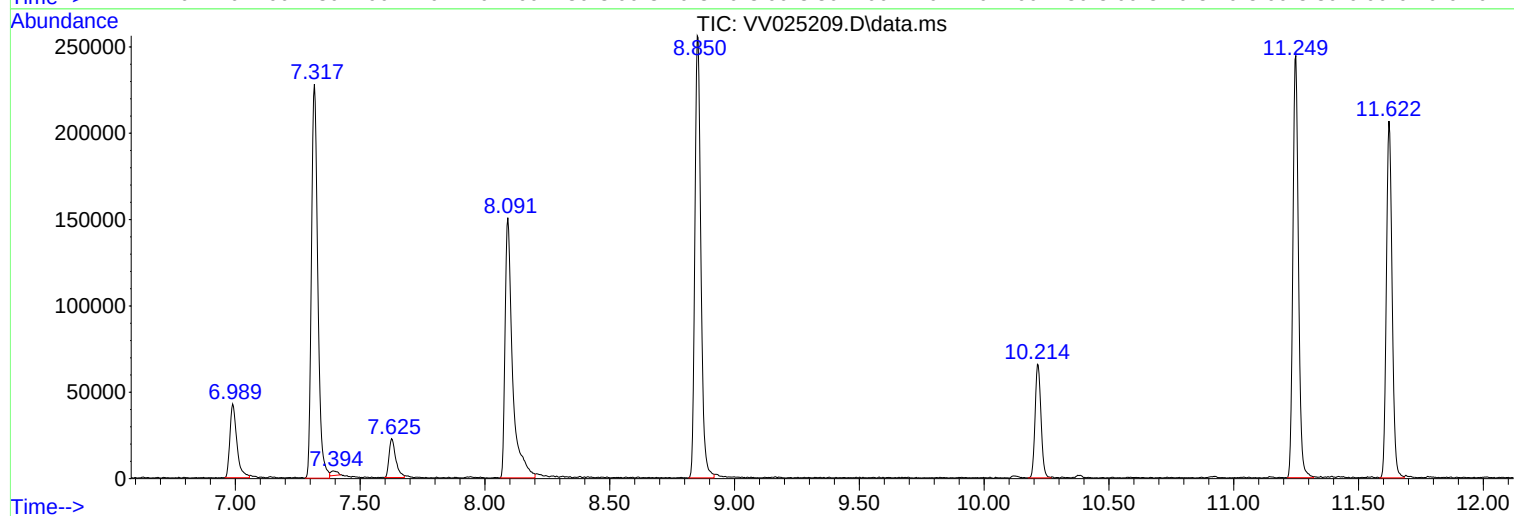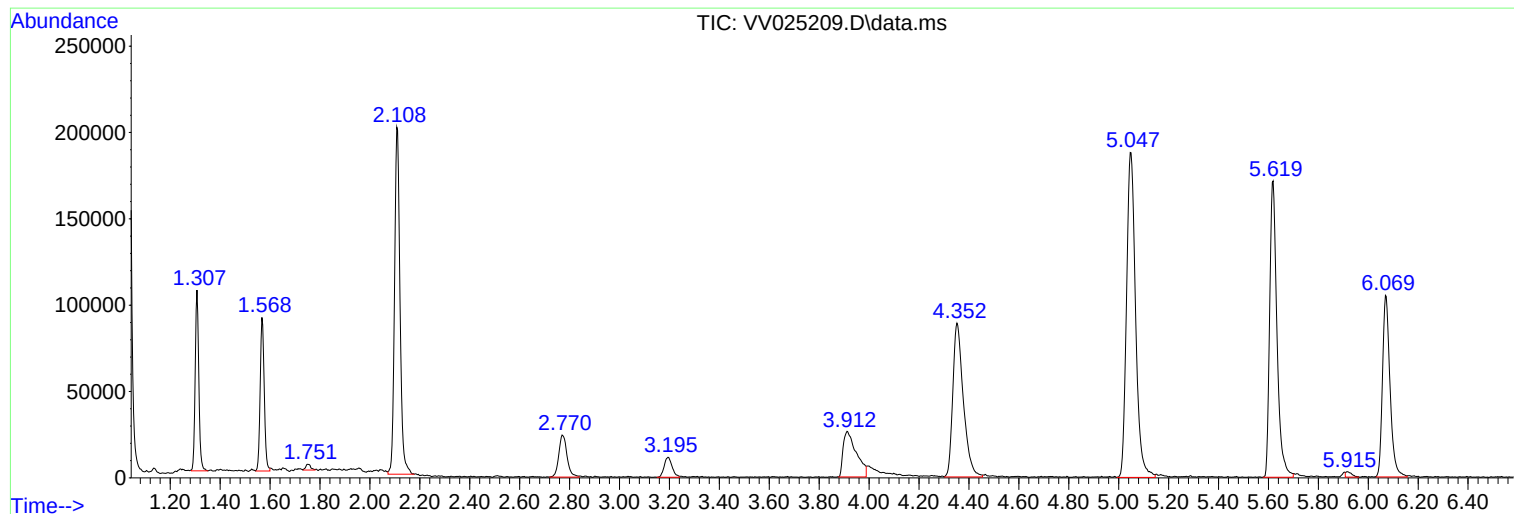

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025209.D
Acq On : 26 Mar 2022 19:33
Operator : SY/MD
Sample : N2097-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025209.D
Acq On : 26 Mar 2022 19:33
Operator : SY/MD
Sample : N2097-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
