

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
 Data File : VV025210.D
 Acq On : 26 Mar 2022 19:56
 Operator : SY/MD
 Sample : N2097-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025210.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rBV	103998	105858	21.69%	2.286%
2	1.571	156	165	173	rBV	91848	103818	21.28%	2.242%
3	1.754	217	222	229	rVB4	4622	5173	1.06%	0.112%
4	2.111	322	333	354	rVB2	258086	436779	89.51%	9.431%
5	2.773	522	539	551	rBV2	11263	24948	5.11%	0.539%
6	3.905	880	891	922	rBV2	32479	120649	24.72%	2.605%
7	4.355	1014	1031	1065	rBV3	102431	333038	68.25%	7.191%
8	4.609	1093	1110	1126	rBV2	31361	80841	16.57%	1.746%
9	5.050	1231	1247	1272	rBV2	196570	487975	100.00%	10.536%
10	5.619	1412	1424	1452	rBV	170726	353733	72.49%	7.638%
11	5.915	1504	1516	1543	rBV2	86563	180292	36.95%	3.893%
12	6.069	1552	1564	1592	rBV2	109522	229285	46.99%	4.951%
13	6.989	1838	1850	1864	rBV2	45106	83491	17.11%	1.803%
14	7.317	1939	1952	1971	rBV	238843	422708	86.62%	9.127%
15	7.625	2038	2048	2064	rBV2	24372	44732	9.17%	0.966%
16	7.979	2150	2158	2169	rVB4	9715	17171	3.52%	0.371%
17	8.088	2183	2192	2231	rBV	158639	324164	66.43%	6.999%
18	8.850	2415	2429	2451	rBV	265529	437671	89.69%	9.450%
19	10.214	2843	2853	2868	rBV	69930	110823	22.71%	2.393%
20	11.246	3163	3174	3193	rBV	243851	387070	79.32%	8.358%
21	11.622	3280	3291	3313	rBV	220088	341088	69.90%	7.365%




Sum of corrected areas: 4631307

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025210.D
Acq On : 26 Mar 2022 19:56
Operator : SY/MD
Sample : N2097-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

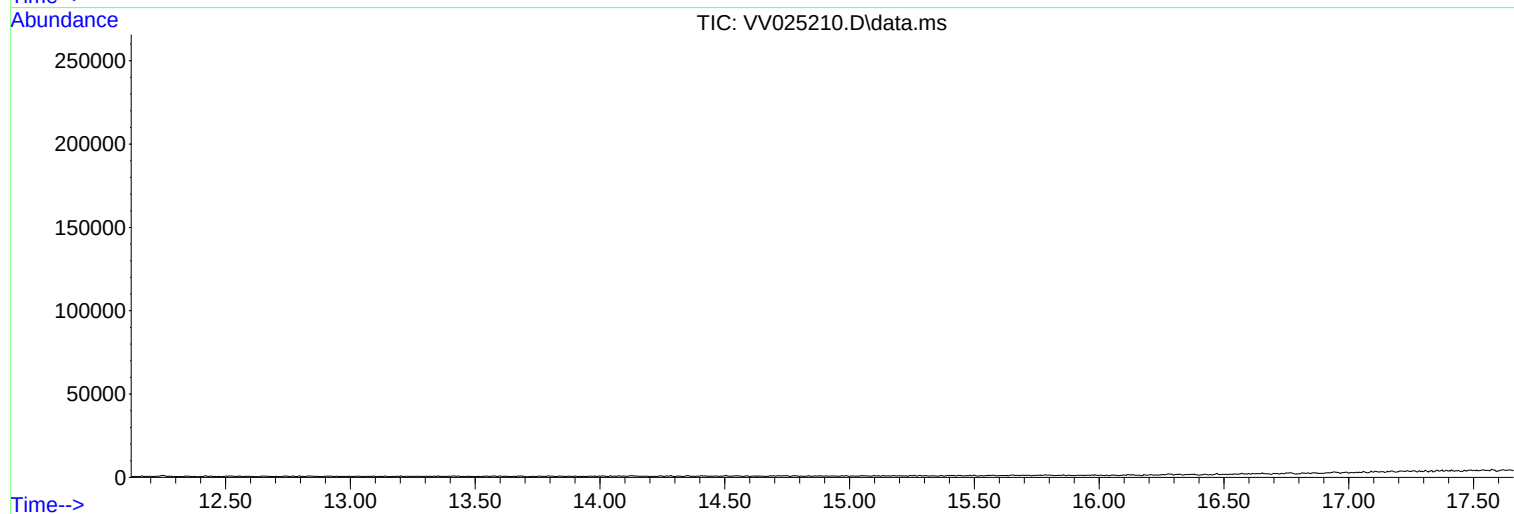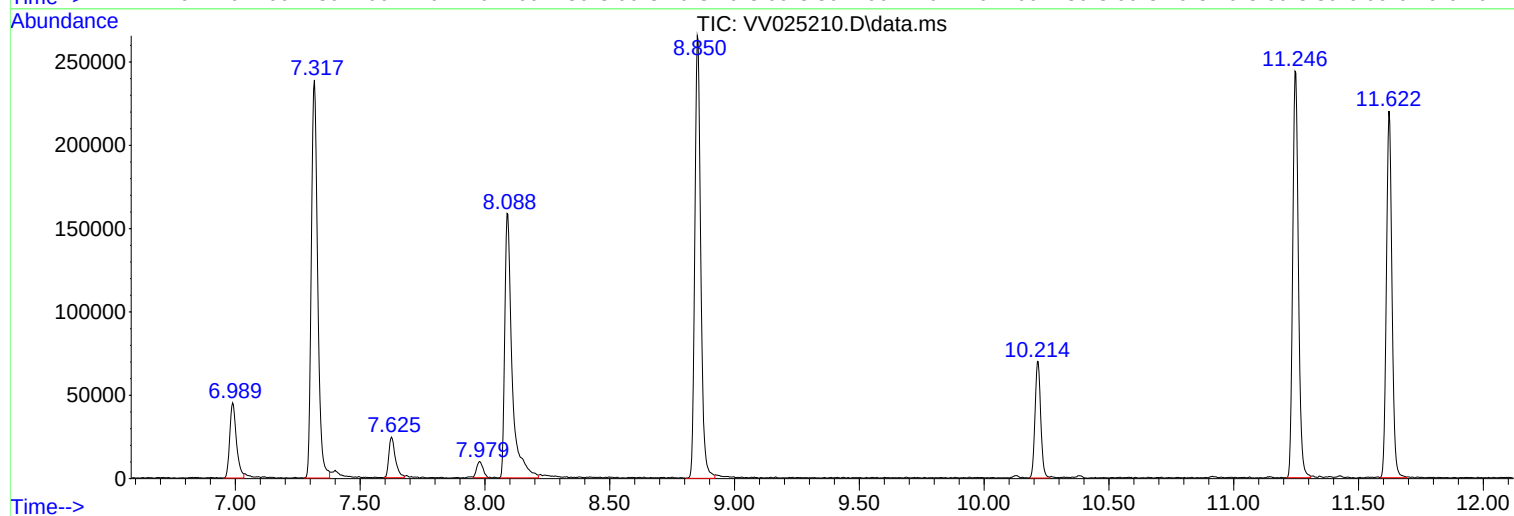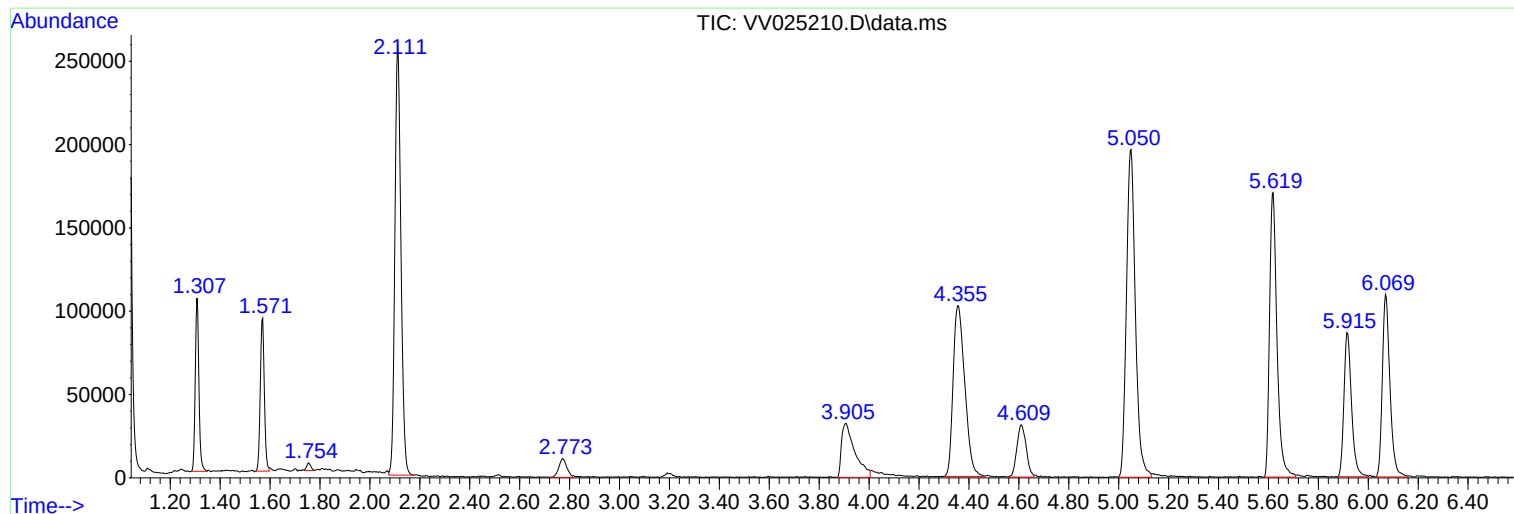

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025210.D
Acq On : 26 Mar 2022 19:56
Operator : SY/MD
Sample : N2097-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025210.D
Acq On : 26 Mar 2022 19:56
Operator : SY/MD
Sample : N2097-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc