

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
 Data File : VV025213.D
 Acq On : 26 Mar 2022 21:07
 Operator : SY/MD
 Sample : N2097-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025213.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	100	rBV	107233	108468	22.04%	2.597%
2	1.568	157	164	173	rBV	90605	104351	21.20%	2.498%
3	2.108	320	332	352	rVB	202775	301679	61.29%	7.222%
4	3.918	884	895	935	rBV2	24578	113939	23.15%	2.728%
5	4.352	1013	1030	1054	rBV	86323	218184	44.32%	5.223%
6	5.050	1232	1247	1273	rBV2	196965	492251	100.00%	11.784%
7	5.619	1412	1424	1447	rBV	172219	355088	72.14%	8.500%
8	5.915	1506	1516	1518	rBV5	3508	4929	1.00%	0.118%
9	6.069	1550	1564	1588	rBV	108816	227737	46.26%	5.452%
10	6.989	1838	1850	1871	rBV	43930	84117	17.09%	2.014%
11	7.317	1940	1952	1972	rBV	240203	423536	86.04%	10.139%
12	7.625	2039	2048	2067	rBV	25025	46211	9.39%	1.106%
13	7.976	2142	2157	2177	rVB2	39309	67735	13.76%	1.621%
14	8.091	2182	2193	2230	rBV	152431	332237	67.49%	7.953%
15	8.850	2418	2429	2452	rBV	268696	443081	90.01%	10.607%
16	10.217	2843	2854	2866	rBV	73148	115867	23.54%	2.774%
17	11.249	3162	3175	3196	rBV	247958	388833	78.99%	9.308%
18	11.542	3258	3266	3274	rBV5	3009	5293	1.08%	0.127%
19	11.622	3280	3291	3308	rBV	219996	343806	69.84%	8.230%




Sum of corrected areas: 4177342

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025213.D
Acq On : 26 Mar 2022 21:07
Operator : SY/MD
Sample : N2097-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

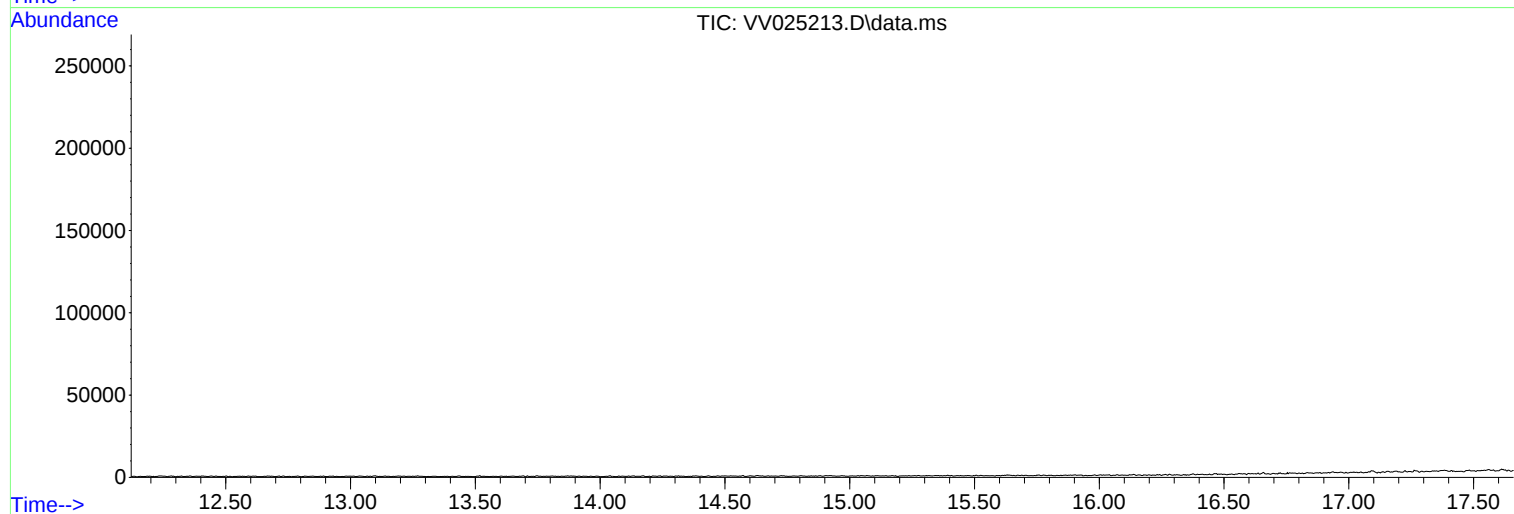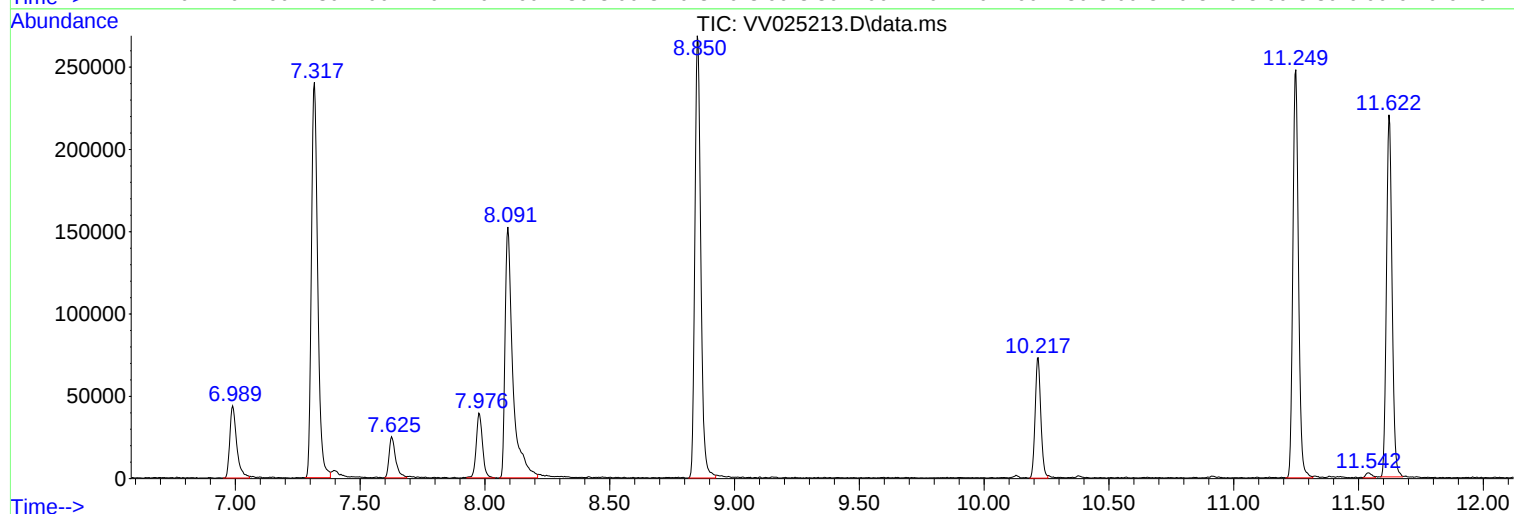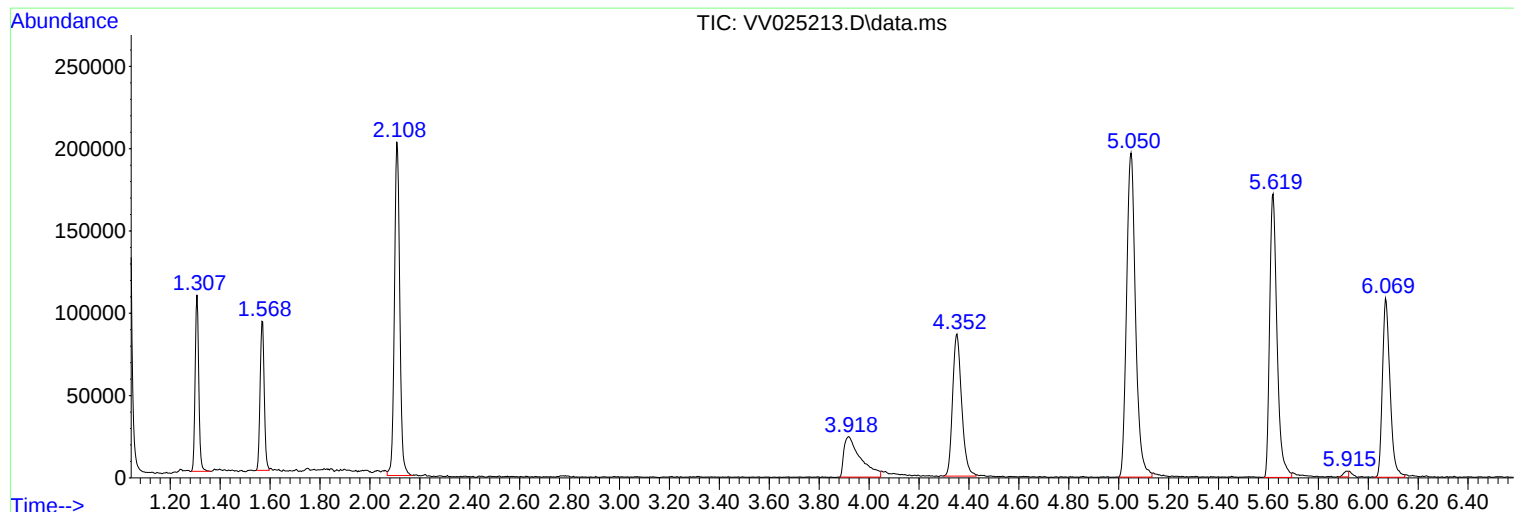

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025213.D
Acq On : 26 Mar 2022 21:07
Operator : SY/MD
Sample : N2097-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025213.D
Acq On : 26 Mar 2022 21:07
Operator : SY/MD
Sample : N2097-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc