

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
 Data File : VV025217.D
 Acq On : 26 Mar 2022 22:40
 Operator : SY/MD
 Sample : N2097-11
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE0

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025217.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	99	rVB	114371	114352	23.23%	2.881%
2	1.568	156	164	175	rBV	97417	110438	22.44%	2.783%
3	2.108	320	332	359	rVB	208716	315507	64.10%	7.950%
4	3.918	884	895	896	rBV	20272	23928	4.86%	0.603%
5	4.352	1016	1030	1057	rVB	85490	215637	43.81%	5.434%
6	5.047	1231	1246	1278	rBV3	194407	492211	100.00%	12.403%
7	5.619	1412	1424	1455	rBV	163750	340847	69.25%	8.589%
8	6.069	1552	1564	1591	rBV2	107696	228150	46.35%	5.749%
9	6.989	1838	1850	1872	rBV	43980	84524	17.17%	2.130%
10	7.317	1940	1952	1970	rBV	234412	415929	84.50%	10.481%
11	7.625	2039	2048	2065	rBV	25163	46341	9.41%	1.168%
12	8.092	2180	2193	2233	rBV	149052	332065	67.46%	8.367%
13	8.850	2418	2429	2449	rBV	252363	421078	85.55%	10.610%
14	10.214	2839	2853	2868	rBV2	72498	115048	23.37%	2.899%
15	11.246	3164	3174	3194	rBV	237570	369617	75.09%	9.314%
16	11.622	3280	3291	3310	rBV	220516	342926	69.67%	8.641%




Sum of corrected areas: 3968598

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025217.D
Acq On : 26 Mar 2022 22:40
Operator : SY/MD
Sample : N2097-11
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

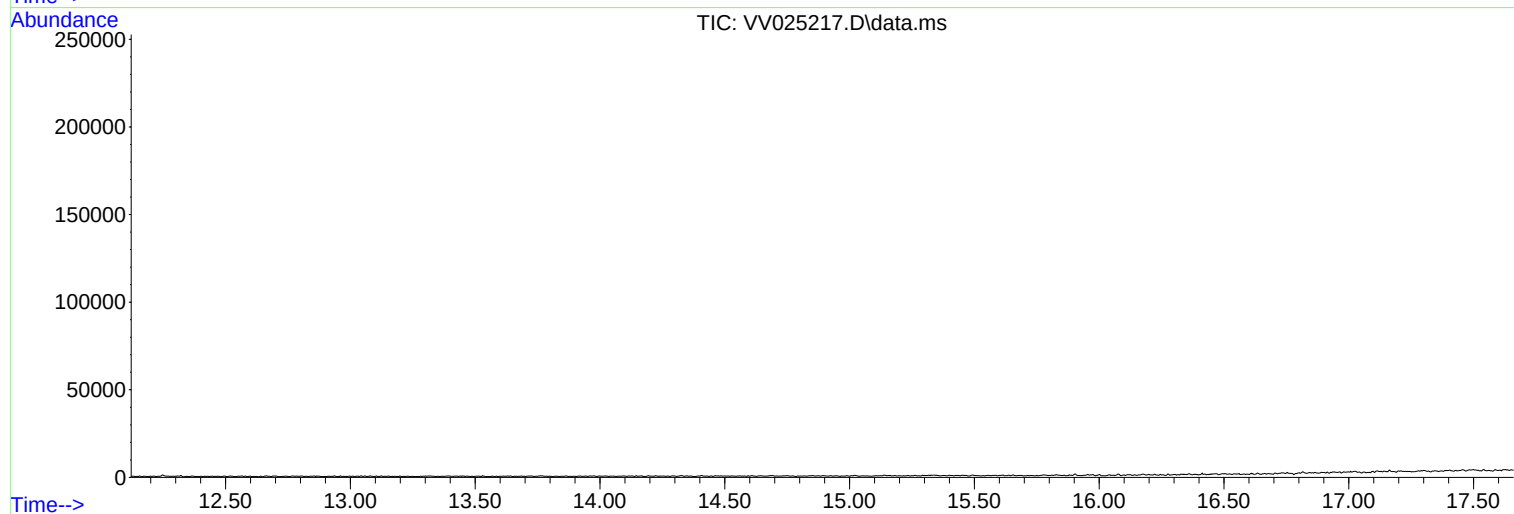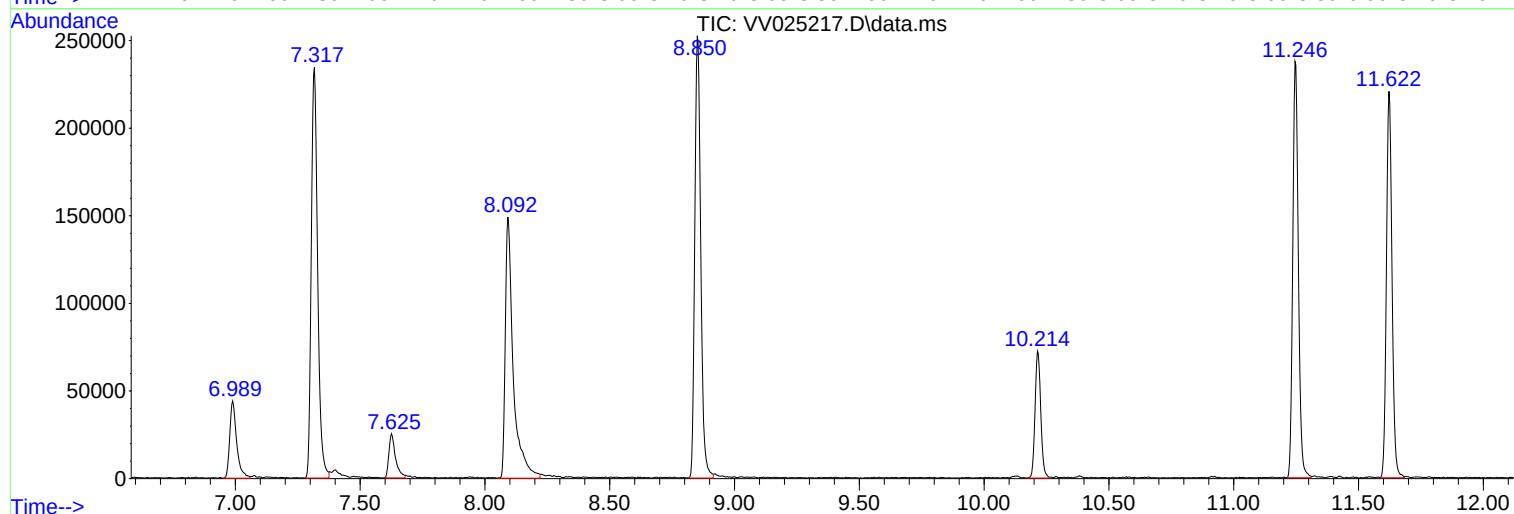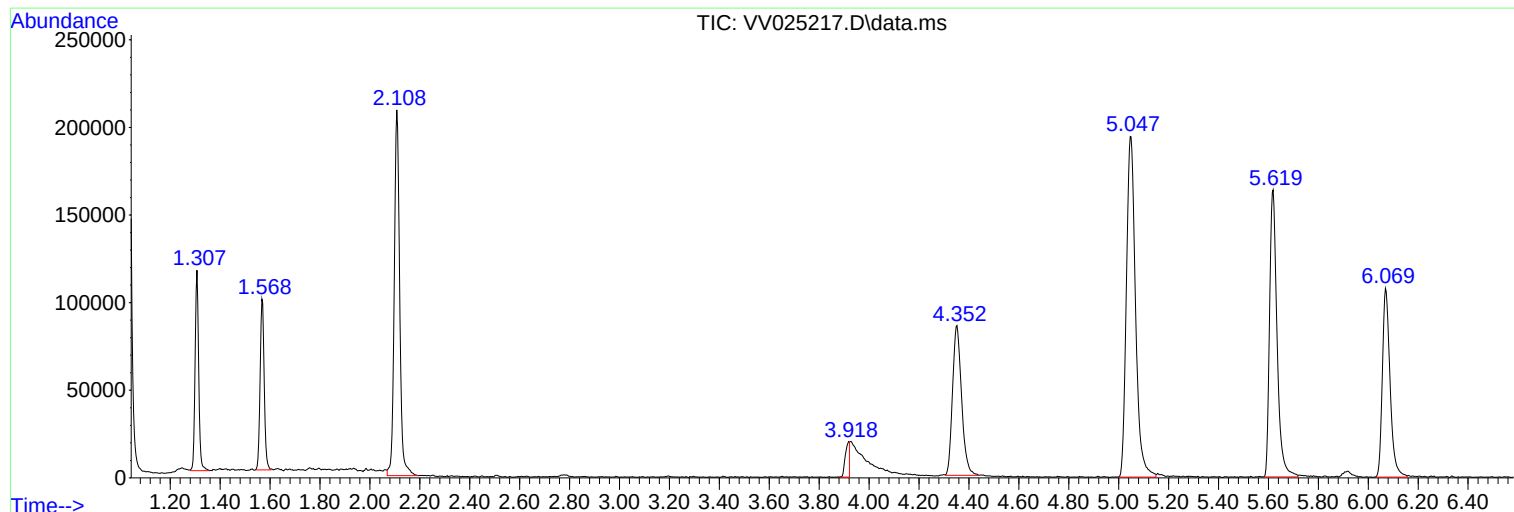

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025217.D
Acq On : 26 Mar 2022 22:40
Operator : SY/MD
Sample : N2097-11
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025217.D
Acq On : 26 Mar 2022 22:40
Operator : SY/MD
Sample : N2097-11
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc