

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
 Data File : VV025218.D
 Acq On : 26 Mar 2022 23:04
 Operator : SY/MD
 Sample : N2097-12
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025218.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	74	83	96	rVB	100174	102225	20.98%	2.246%
2	1.462	127	131	135	rBV	12501	8292	1.70%	0.182%
3	1.571	157	165	177	rBV	86488	101325	20.80%	2.226%
4	2.111	322	333	353	rVB2	227292	364221	74.76%	8.003%
5	2.773	523	539	554	rBV3	16857	37469	7.69%	0.823%
6	3.198	659	671	680	rBV4	4187	8323	1.71%	0.183%
7	3.908	879	892	932	rBV	31185	125511	25.76%	2.758%
8	4.355	1014	1031	1059	rBV5	94849	297784	61.13%	6.543%
9	4.613	1093	1111	1132	rVB2	28456	70574	14.49%	1.551%
10	5.050	1230	1247	1271	rBV2	195370	487168	100.00%	10.705%
11	5.619	1413	1424	1450	rBV	167245	344297	70.67%	7.566%
12	5.918	1504	1517	1552	rVB	91288	192358	39.48%	4.227%
13	6.069	1552	1564	1591	rBV2	110203	227588	46.72%	5.001%
14	6.989	1840	1850	1871	rBV2	42858	82560	16.95%	1.814%
15	7.317	1941	1952	1970	rBV	236225	417610	85.72%	9.176%
16	7.397	1970	1977	1990	rVB3	8654	16957	3.48%	0.373%
17	7.625	2039	2048	2068	rBV	24929	44979	9.23%	0.988%
18	7.979	2149	2158	2172	rVB4	12049	21228	4.36%	0.466%
19	8.092	2183	2193	2230	rBV	156874	330545	67.85%	7.263%
20	8.850	2418	2429	2450	rBV	263441	429145	88.09%	9.430%
21	10.217	2841	2854	2868	rBV	71076	114117	23.42%	2.508%
22	11.246	3159	3174	3200	rBV	240878	380980	78.20%	8.372%
23	11.622	3280	3291	3316	rBV	214804	340253	69.84%	7.477%
24	16.307	4740	4748	4755	rBV7	3816	5371	1.10%	0.118%




Sum of corrected areas: 4550880

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025218.D
Acq On : 26 Mar 2022 23:04
Operator : SY/MD
Sample : N2097-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

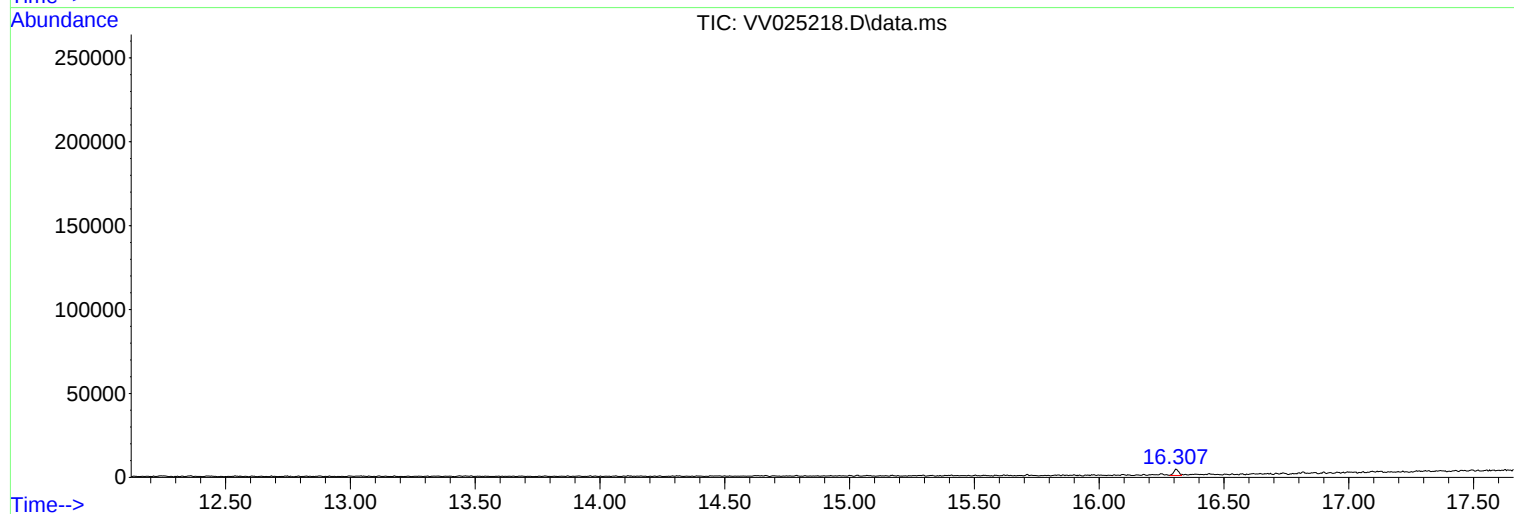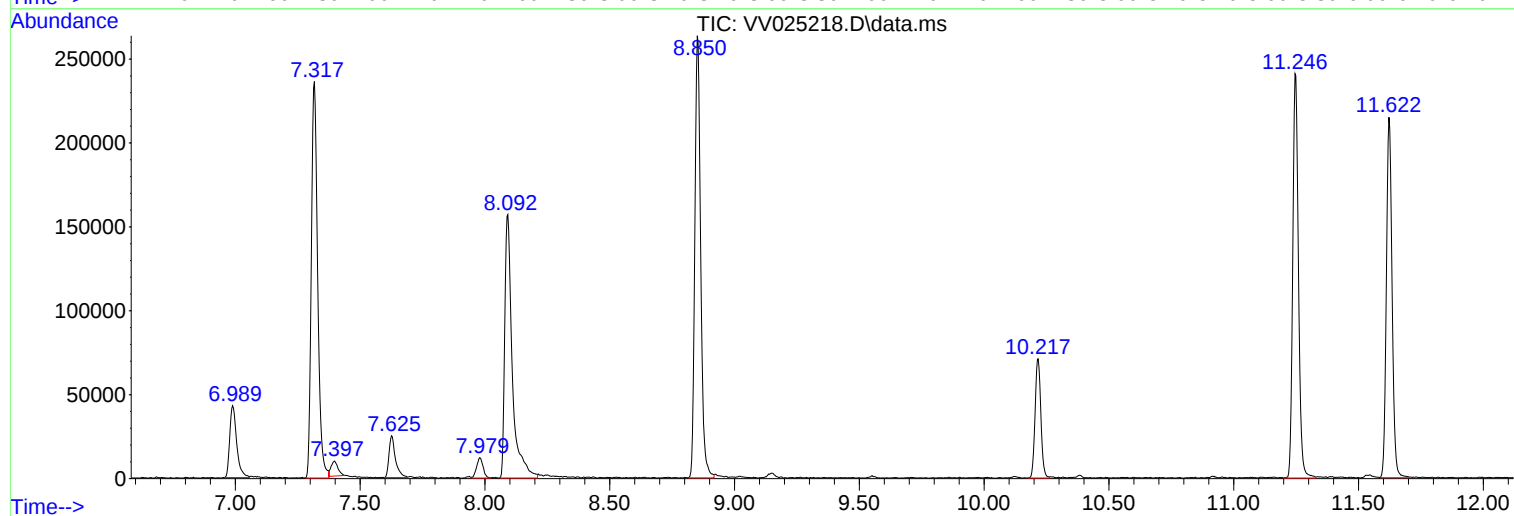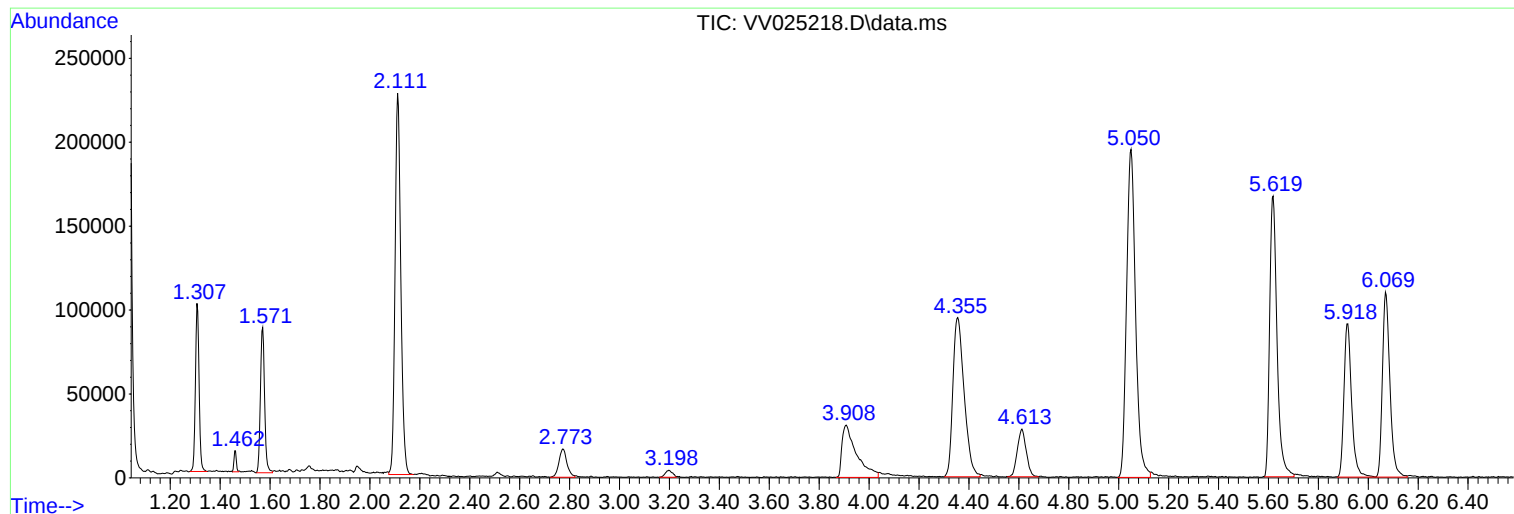

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025218.D
Acq On : 26 Mar 2022 23:04
Operator : SY/MD
Sample : N2097-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025218.D
Acq On : 26 Mar 2022 23:04
Operator : SY/MD
Sample : N2097-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc