

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
 Data File : VV025219.D
 Acq On : 26 Mar 2022 23:27
 Operator : SY/MD
 Sample : N2097-13
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025219.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	93	rVB	105273	106498	21.49%	2.221%
2	1.571	157	165	178	rBV	88129	102328	20.65%	2.134%
3	2.111	322	333	349	rBV	196758	287439	58.01%	5.994%
4	2.198	349	360	361	rBV	13194	17295	3.49%	0.361%
5	3.918	883	895	924	rBV	27335	116943	23.60%	2.439%
6	4.352	1013	1030	1056	rBV	86122	218683	44.14%	4.560%
7	5.050	1230	1247	1272	rBV2	195464	495471	100.00%	10.332%
8	5.619	1412	1424	1446	rBV	168524	348673	70.37%	7.271%
9	5.912	1506	1515	1528	rBV8	3884	8200	1.65%	0.171%
10	6.069	1551	1564	1588	rBV	110175	228872	46.19%	4.773%
11	6.989	1840	1850	1866	rBV	45604	84806	17.12%	1.768%
12	7.317	1940	1952	1964	rBV	240985	421576	85.09%	8.791%
13	7.387	1964	1974	1996	rVB	218238	380931	76.88%	7.944%
14	7.625	2039	2048	2062	rBV	24635	45354	9.15%	0.946%
15	8.092	2179	2193	2227	rBV	156866	332947	67.20%	6.943%
16	8.850	2419	2429	2453	rBV	261910	433633	87.52%	9.043%
17	9.014	2470	2480	2494	rBV	31277	51848	10.46%	1.081%
18	9.137	2507	2518	2539	rBV	116692	202111	40.79%	4.215%
19	9.545	2636	2645	2659	rBV	38886	61245	12.36%	1.277%
20	10.214	2843	2853	2868	rBV	71550	114319	23.07%	2.384%
21	11.249	3160	3175	3191	rBV	253025	384786	77.66%	8.024%
22	11.622	3278	3291	3310	rBV	218241	351537	70.95%	7.331%




Sum of corrected areas: 4795495

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025219.D
Acq On : 26 Mar 2022 23:27
Operator : SY/MD
Sample : N2097-13
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

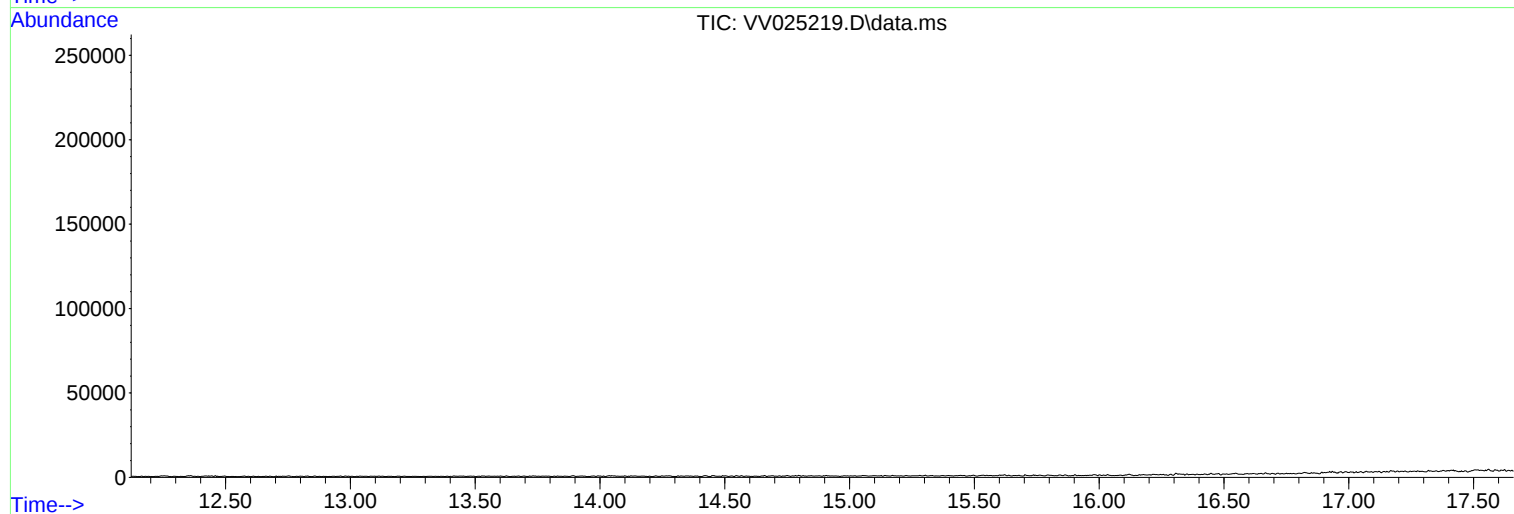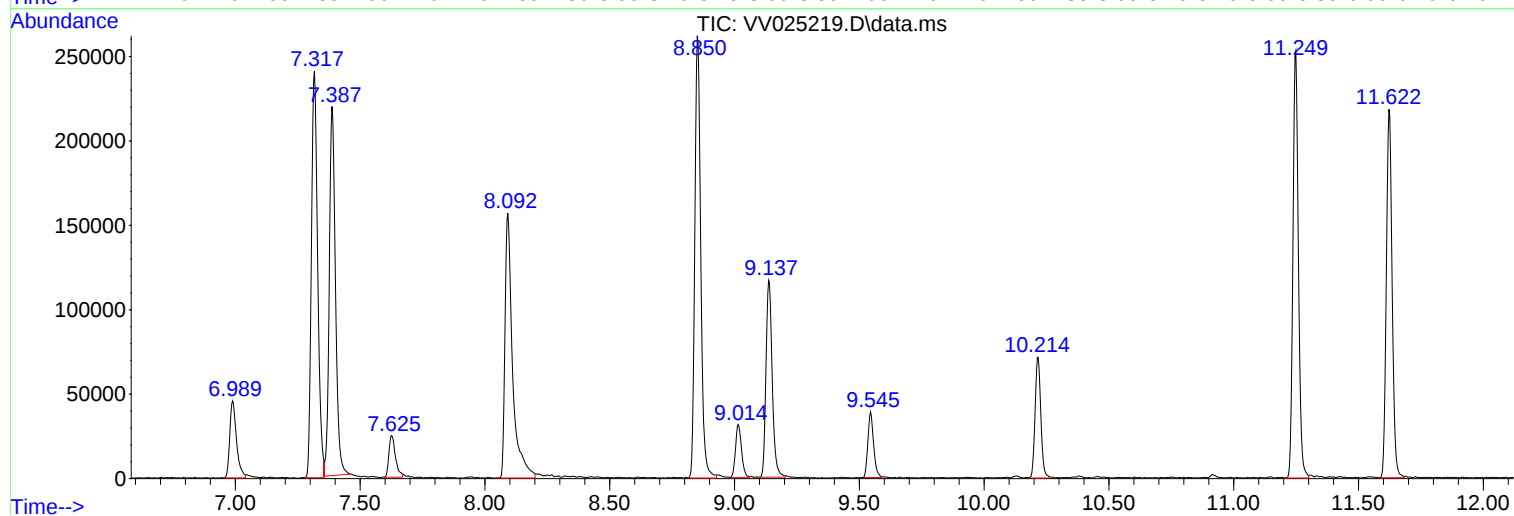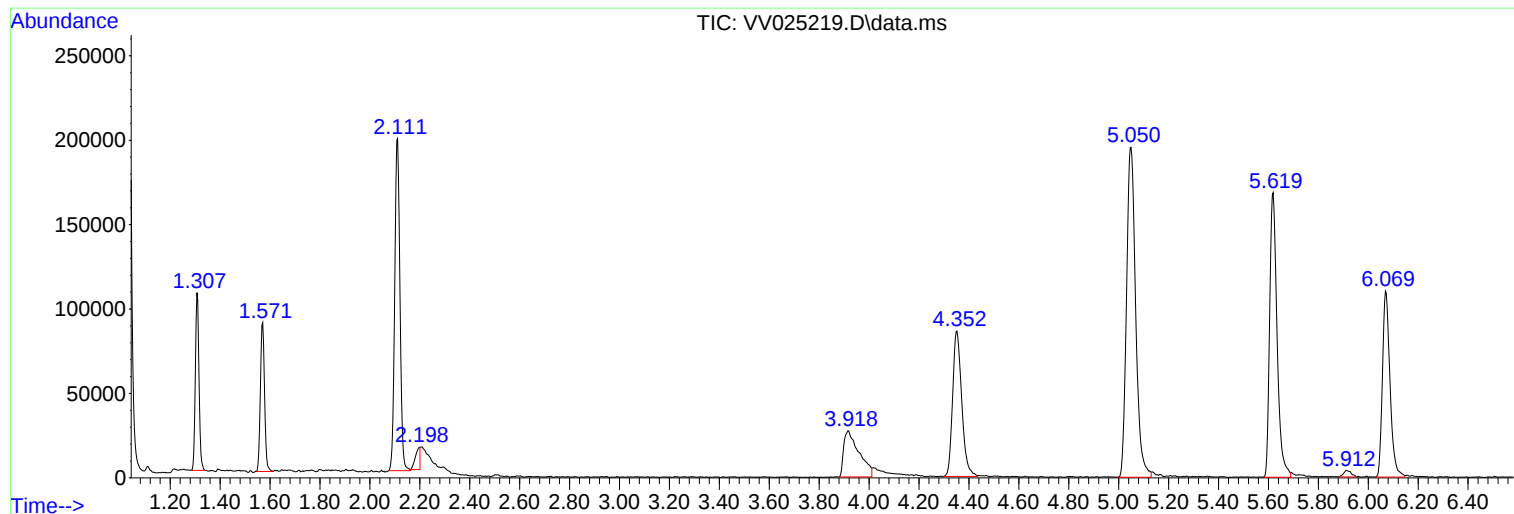

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025219.D
Acq On : 26 Mar 2022 23:27
Operator : SY/MD
Sample : N2097-13
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025219.D
Acq On : 26 Mar 2022 23:27
Operator : SY/MD
Sample : N2097-13
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------