

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
 Data File : VV025220.D
 Acq On : 26 Mar 2022 23:51
 Operator : SY/MD
 Sample : N2097-14
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025220.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB	103975	105259	22.61%	2.472%
2	1.568	157	164	179	rVB	87269	100052	21.49%	2.350%
3	2.108	321	332	351	rVB	191177	279822	60.10%	6.572%
4	2.204	353	362	365	rBV	4754	7569	1.63%	0.178%
5	3.924	884	897	936	rBV2	22993	113341	24.34%	2.662%
6	4.352	1014	1030	1055	rBV3	81692	206662	44.38%	4.854%
7	5.050	1231	1247	1278	rBV2	186250	465624	100.00%	10.937%
8	5.619	1413	1424	1445	rBV	161304	333451	71.61%	7.832%
9	5.911	1510	1515	1526	rVB6	3826	5625	1.21%	0.132%
10	6.069	1553	1564	1589	rBV2	99532	210352	45.18%	4.941%
11	6.989	1840	1850	1869	rBV2	42194	80226	17.23%	1.884%
12	7.317	1941	1952	1965	rBV	224355	394699	84.77%	9.271%
13	7.387	1965	1974	1996	rVB	122564	220183	47.29%	5.172%
14	7.625	2038	2048	2068	rBV	24498	44761	9.61%	1.051%
15	8.091	2183	2193	2222	rBV	143417	305366	65.58%	7.172%
16	8.850	2418	2429	2454	rBV	252553	415377	89.21%	9.756%
17	9.014	2472	2480	2492	rBV	17002	28454	6.11%	0.668%
18	9.140	2507	2519	2537	rBV	64475	110615	23.76%	2.598%
19	9.545	2634	2645	2658	rBV3	19148	32485	6.98%	0.763%
20	10.214	2842	2853	2866	rBV2	66374	106976	22.97%	2.513%
21	11.249	3164	3175	3197	rBV	234736	367001	78.82%	8.620%
22	11.622	3280	3291	3309	rBV	205289	323586	69.50%	7.600%




Sum of corrected areas: 4257486

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025220.D
Acq On : 26 Mar 2022 23:51
Operator : SY/MD
Sample : N2097-14
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

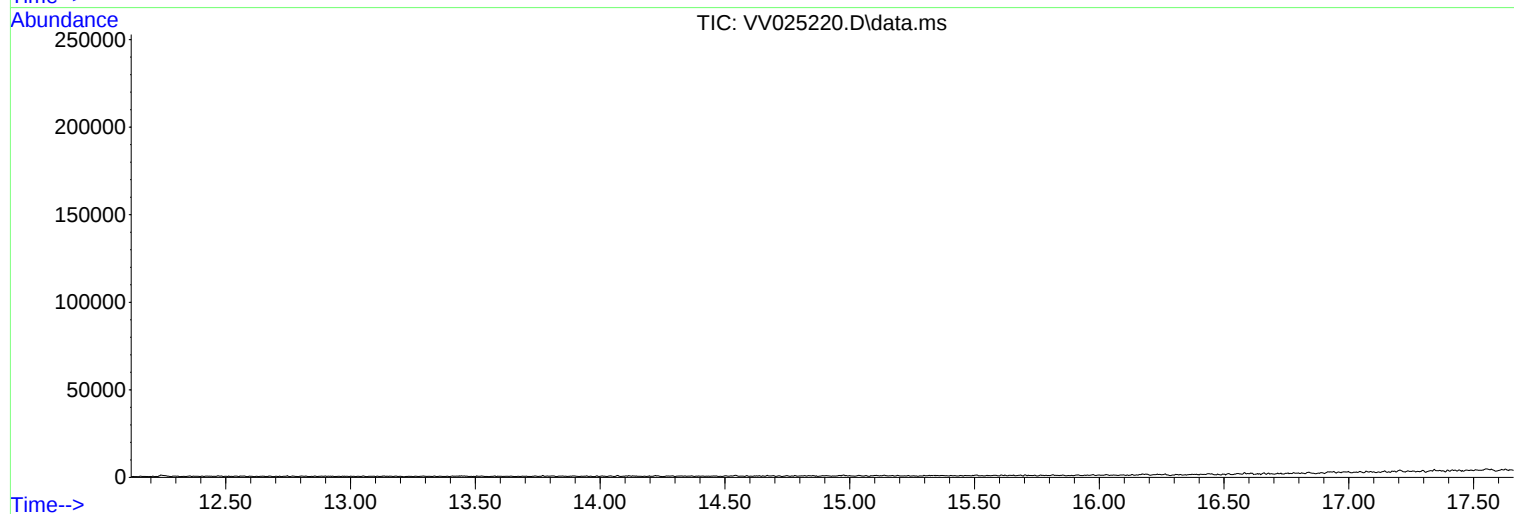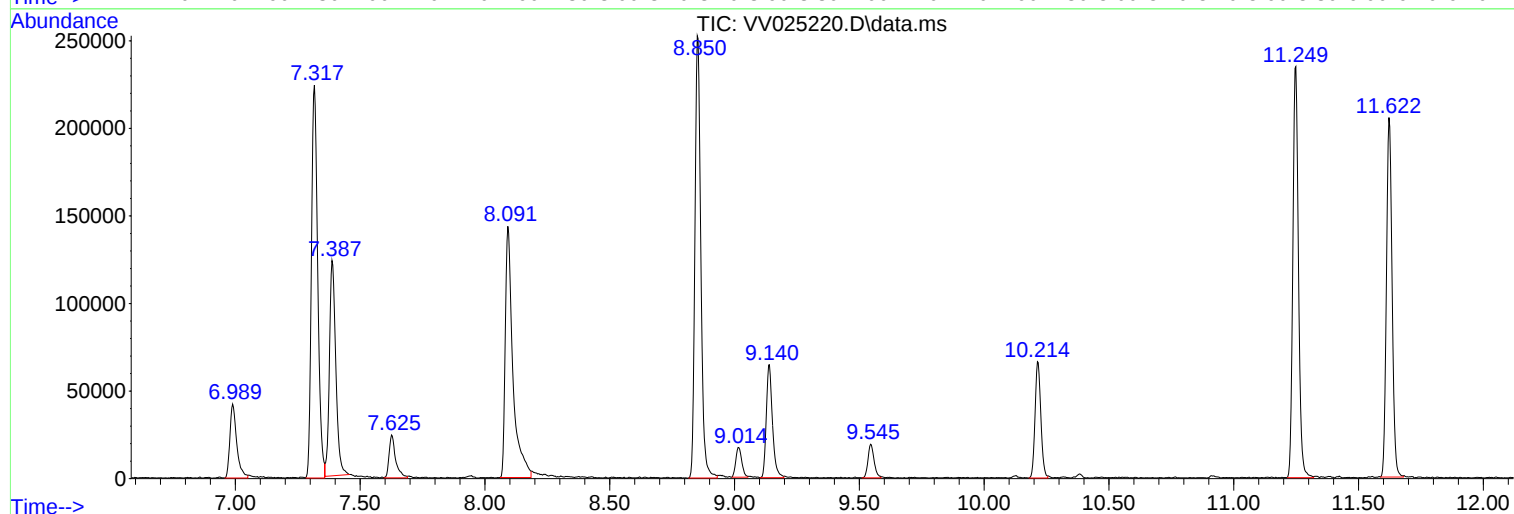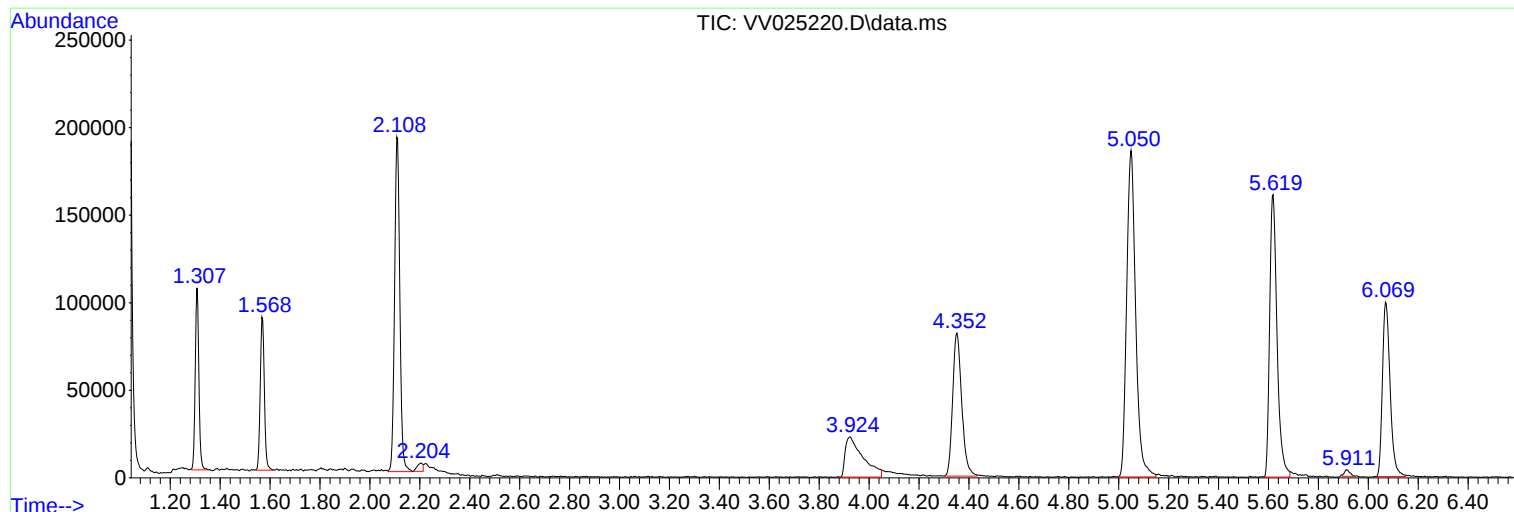

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025220.D
Acq On : 26 Mar 2022 23:51
Operator : SY/MD
Sample : N2097-14
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025220.D
Acq On : 26 Mar 2022 23:51
Operator : SY/MD
Sample : N2097-14
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
