

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
 Data File : VV025224.D
 Acq On : 27 Mar 2022 01:48
 Operator : SY/MD
 Sample : N2097-16
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025224.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	92	rVB	115566	112374	22.90%	2.772%
2	1.568	156	164	175	rBV	96105	110317	22.48%	2.722%
3	2.108	322	332	354	rVB	206759	309505	63.07%	7.636%
4	2.773	522	539	557	rBV2	20724	46240	9.42%	1.141%
5	3.921	884	896	899	rBV2	20397	34764	7.08%	0.858%
6	4.352	1012	1030	1059	rBV3	85349	220408	44.91%	5.438%
7	5.050	1230	1247	1275	rBV2	198185	490725	100.00%	12.107%
8	5.619	1412	1424	1448	rBV	167265	349316	71.18%	8.618%
9	5.915	1507	1516	1531	rBV8	3518	8027	1.64%	0.198%
10	6.069	1551	1564	1585	rBV	108650	227433	46.35%	5.611%
11	6.989	1838	1850	1875	rBV2	42573	84162	17.15%	2.076%
12	7.317	1940	1952	1971	rBV	238347	419054	85.39%	10.339%
13	7.397	1973	1977	1991	rVB5	4030	8052	1.64%	0.199%
14	7.625	2039	2048	2069	rBV	23157	44432	9.05%	1.096%
15	8.092	2183	2193	2229	rBV2	143245	325344	66.30%	8.027%
16	8.850	2417	2429	2453	rBV	262769	433412	88.32%	10.693%
17	10.217	2842	2854	2869	rBV2	69962	112659	22.96%	2.779%
18	11.249	3163	3175	3196	rBV	241816	378975	77.23%	9.350%
19	11.622	3277	3291	3308	rBV	210510	338112	68.90%	8.342%




Sum of corrected areas: 4053311

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025224.D
Acq On : 27 Mar 2022 01:48
Operator : SY/MD
Sample : N2097-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

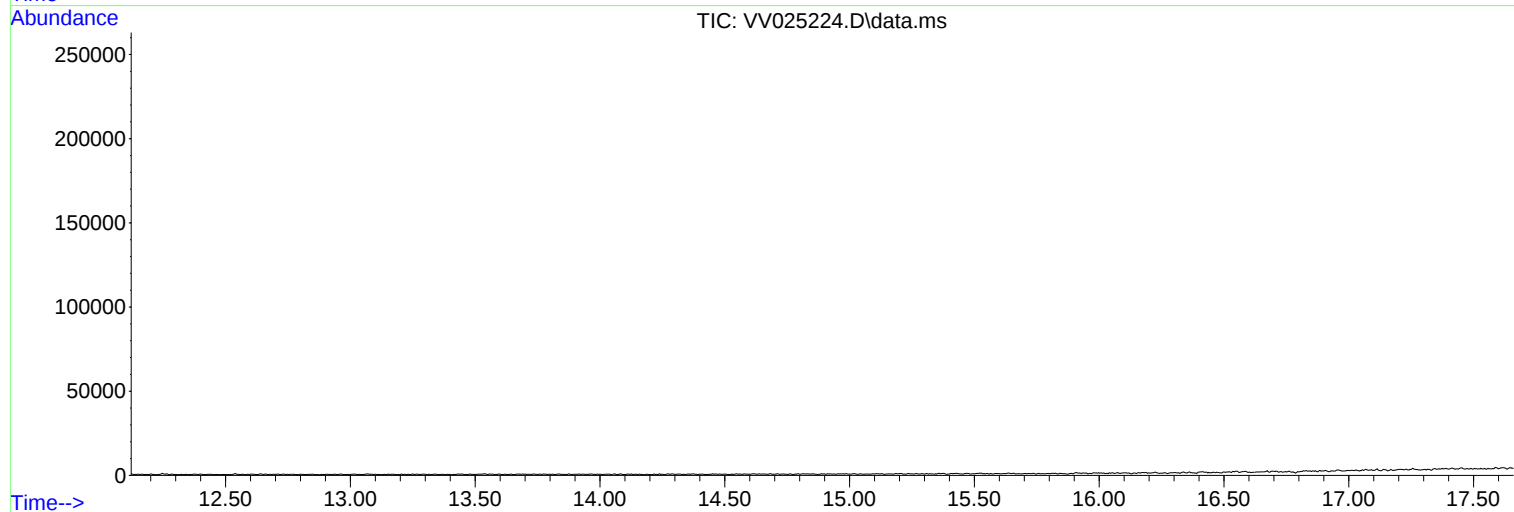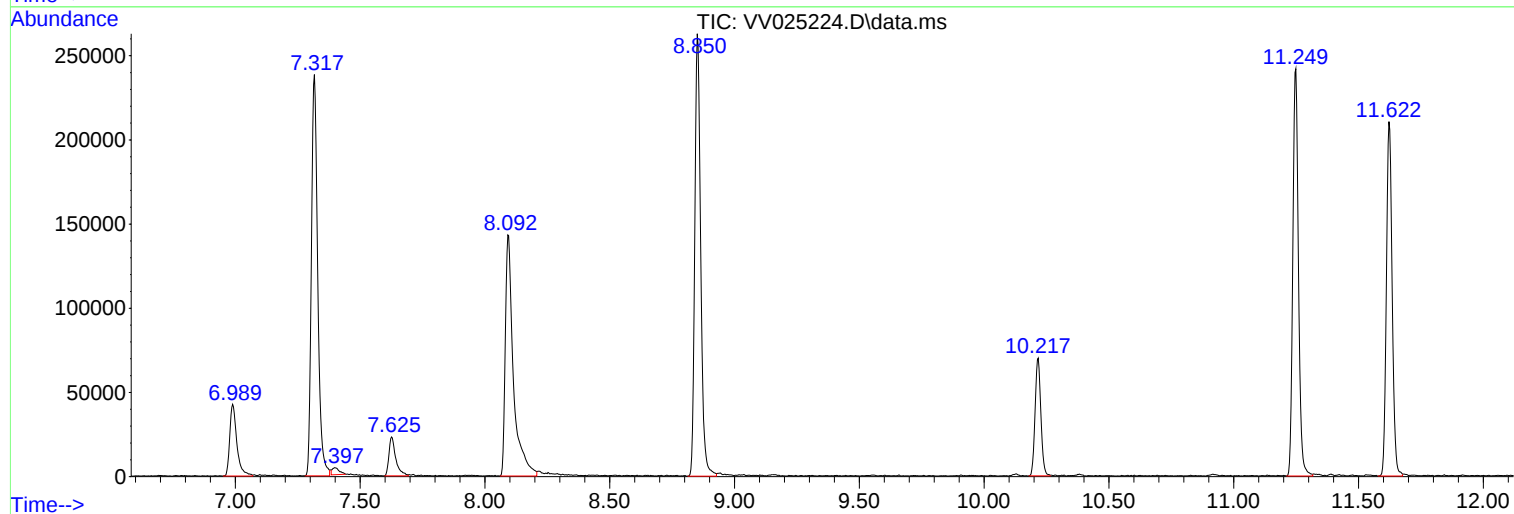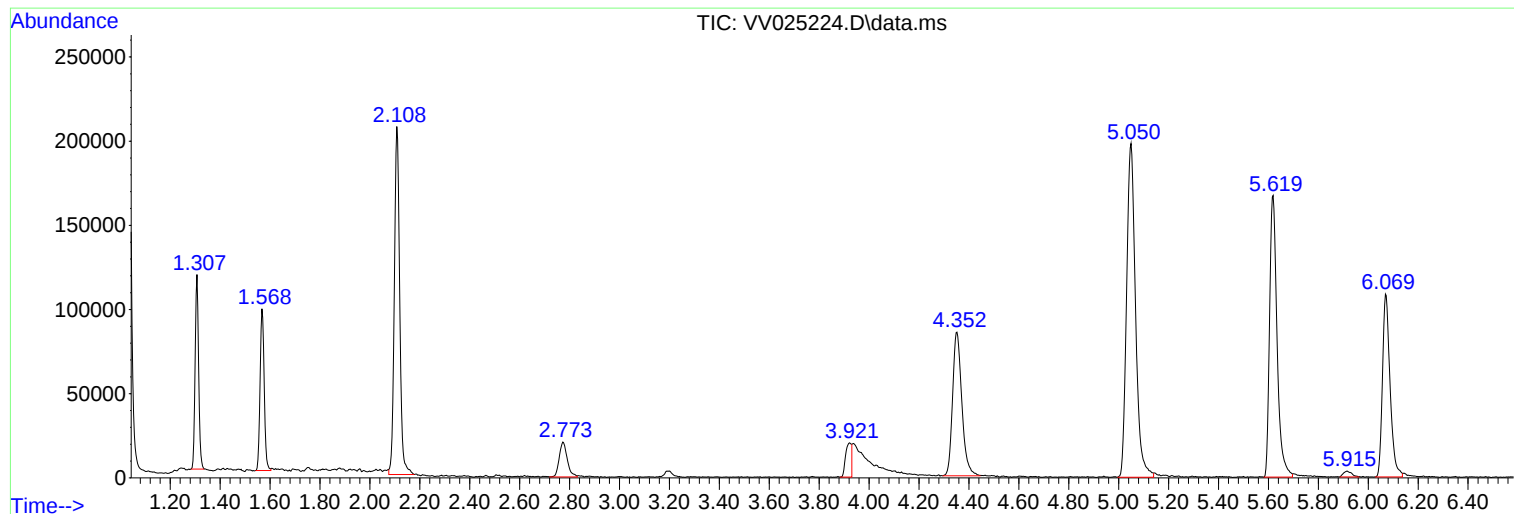

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025224.D
Acq On : 27 Mar 2022 01:48
Operator : SY/MD
Sample : N2097-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025224.D
Acq On : 27 Mar 2022 01:48
Operator : SY/MD
Sample : N2097-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc