

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
 Data File : VV025226.D
 Acq On : 27 Mar 2022 02:34
 Operator : SY/MD
 Sample : N2097-18
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025226.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.124	21	26	34	rVB2	5211	6202	1.27%	0.153%
2	1.307	76	83	99	rVB	107660	108527	22.22%	2.680%
3	1.568	157	164	176	rBV	94262	107872	22.09%	2.664%
4	2.108	321	332	354	rVB	201686	302925	62.03%	7.481%
5	3.921	884	896	940	rBV2	24056	121902	24.96%	3.011%
6	4.352	1013	1030	1056	rBV	85115	220621	45.17%	5.449%
7	5.050	1231	1247	1270	rBV2	197222	488381	100.00%	12.062%
8	5.616	1410	1423	1449	rBV	166363	342045	70.04%	8.448%
9	5.912	1506	1515	1528	rBV7	3801	7893	1.62%	0.195%
10	6.072	1551	1565	1591	rBV	106251	225820	46.24%	5.577%
11	6.989	1837	1850	1871	rBV2	44381	82979	16.99%	2.049%
12	7.317	1938	1952	1971	rBV	236045	421651	86.34%	10.414%
13	7.397	1972	1977	1992	rVB5	4423	9123	1.87%	0.225%
14	7.625	2040	2048	2068	rBV2	23151	45646	9.35%	1.127%
15	8.092	2181	2193	2226	rBV	144546	316408	64.79%	7.814%
16	8.850	2418	2429	2453	rBV	254168	425024	87.03%	10.497%
17	10.217	2842	2854	2869	rBV	68585	111313	22.79%	2.749%
18	11.246	3163	3174	3196	rBV	235568	366280	75.00%	9.046%
19	11.622	3280	3291	3310	rBV	211565	338382	69.29%	8.357%




Sum of corrected areas: 4048994

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025226.D
Acq On : 27 Mar 2022 02:34
Operator : SY/MD
Sample : N2097-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

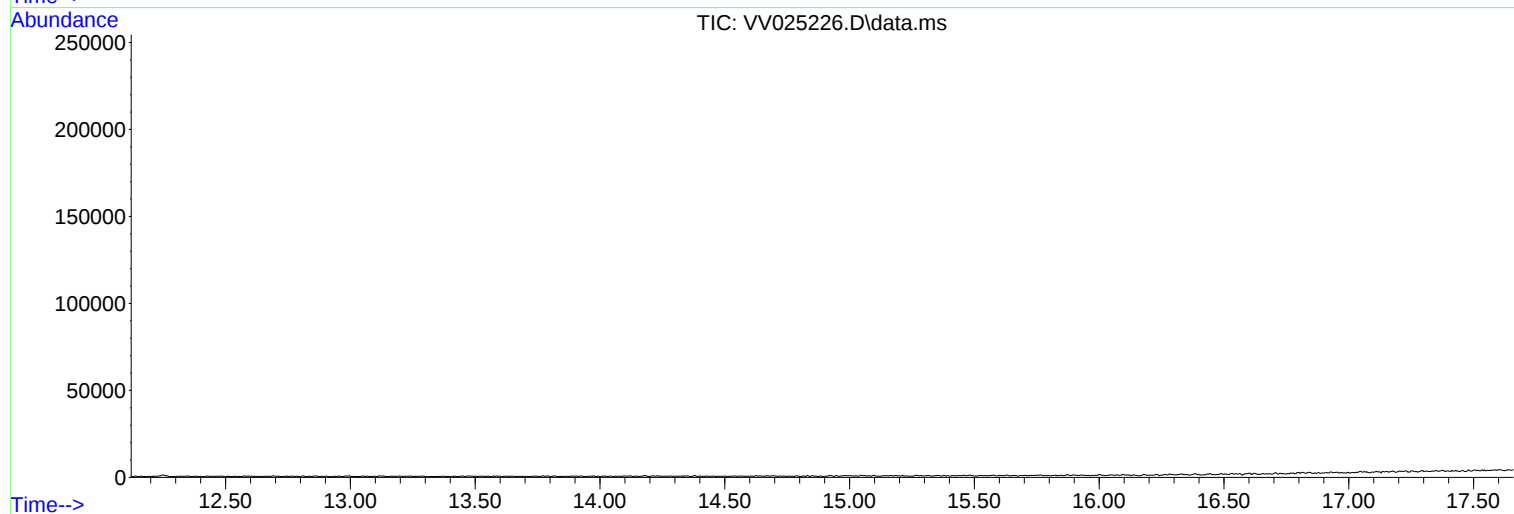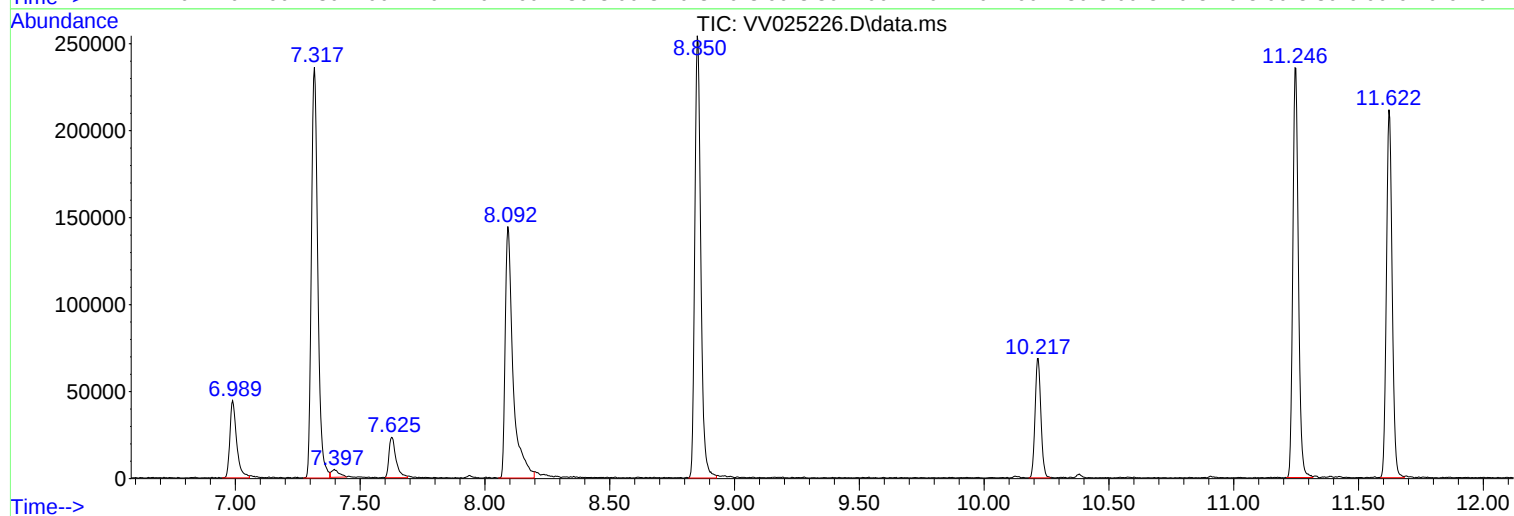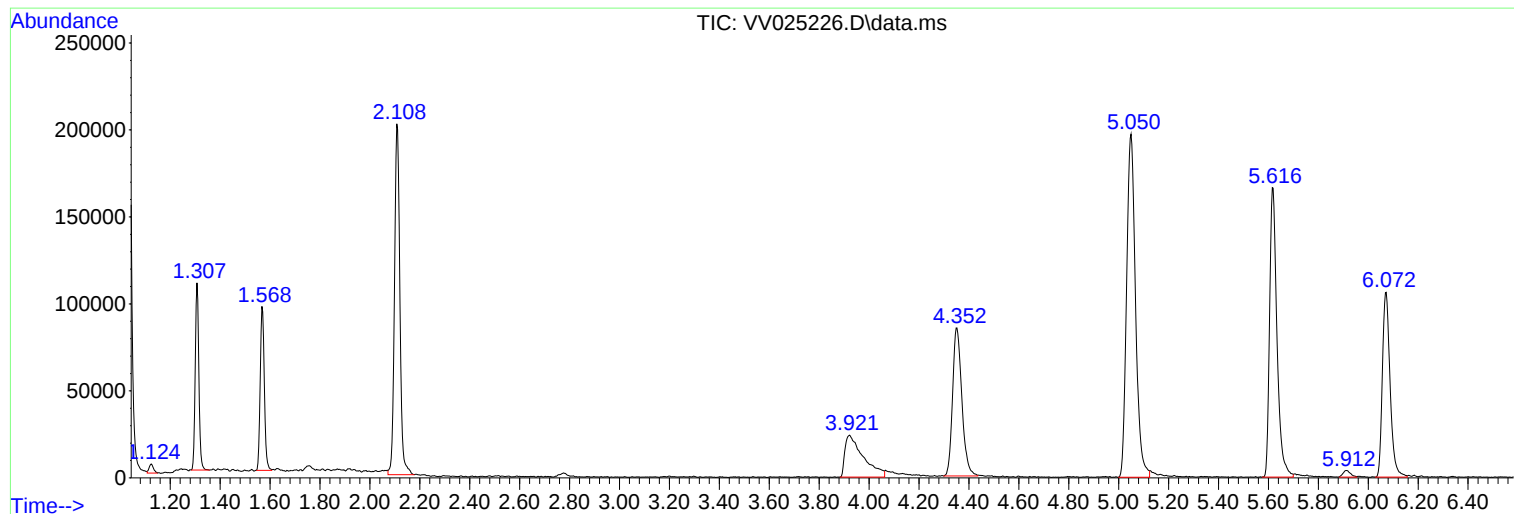

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025226.D
Acq On : 27 Mar 2022 02:34
Operator : SY/MD
Sample : N2097-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025226.D
Acq On : 27 Mar 2022 02:34
Operator : SY/MD
Sample : N2097-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc