

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
 Data File : VV025228.D
 Acq On : 27 Mar 2022 03:21
 Operator : SY/MD
 Sample : N2097-20
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025228.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	94	rVB	105240	104667	21.35%	2.456%
2	1.571	157	165	177	rBV	89485	103157	21.04%	2.421%
3	1.757	214	223	230	rBV	4978	7358	1.50%	0.173%
4	2.111	322	333	357	rVB	197457	296552	60.48%	6.959%
5	2.773	524	539	558	rBV	39247	85822	17.50%	2.014%
6	3.198	657	671	683	rBV3	5877	12764	2.60%	0.300%
7	3.915	884	894	929	rBV2	25693	109905	22.41%	2.579%
8	4.352	1014	1030	1056	rBV2	88759	238324	48.61%	5.592%
9	5.050	1231	1247	1275	rBV2	198110	490321	100.00%	11.505%
10	5.619	1409	1424	1444	rBV	163641	336457	68.62%	7.895%
11	5.918	1503	1517	1530	rBV8	12848	28946	5.90%	0.679%
12	6.069	1552	1564	1586	rBV2	109357	227925	46.48%	5.348%
13	6.989	1838	1850	1874	rBV2	42980	84202	17.17%	1.976%
14	7.317	1935	1952	1970	rBV	235945	412539	84.14%	9.680%
15	7.397	1974	1977	1990	rVB7	3654	5876	1.20%	0.138%
16	7.625	2038	2048	2067	rBV	25058	46600	9.50%	1.093%
17	7.976	2146	2157	2175	rVB	60211	102253	20.85%	2.399%
18	8.092	2183	2193	2223	rBV	150062	322145	65.70%	7.559%
19	8.850	2418	2429	2451	rBV	255133	426197	86.92%	10.001%
20	10.214	2843	2853	2872	rBV	69208	112225	22.89%	2.633%
21	11.249	3163	3175	3196	rBV	240868	368681	75.19%	8.651%
22	11.622	3280	3291	3308	rBV	211121	338779	69.09%	7.949%




Sum of corrected areas: 4261695

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025228.D
Acq On : 27 Mar 2022 03:21
Operator : SY/MD
Sample : N2097-20
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

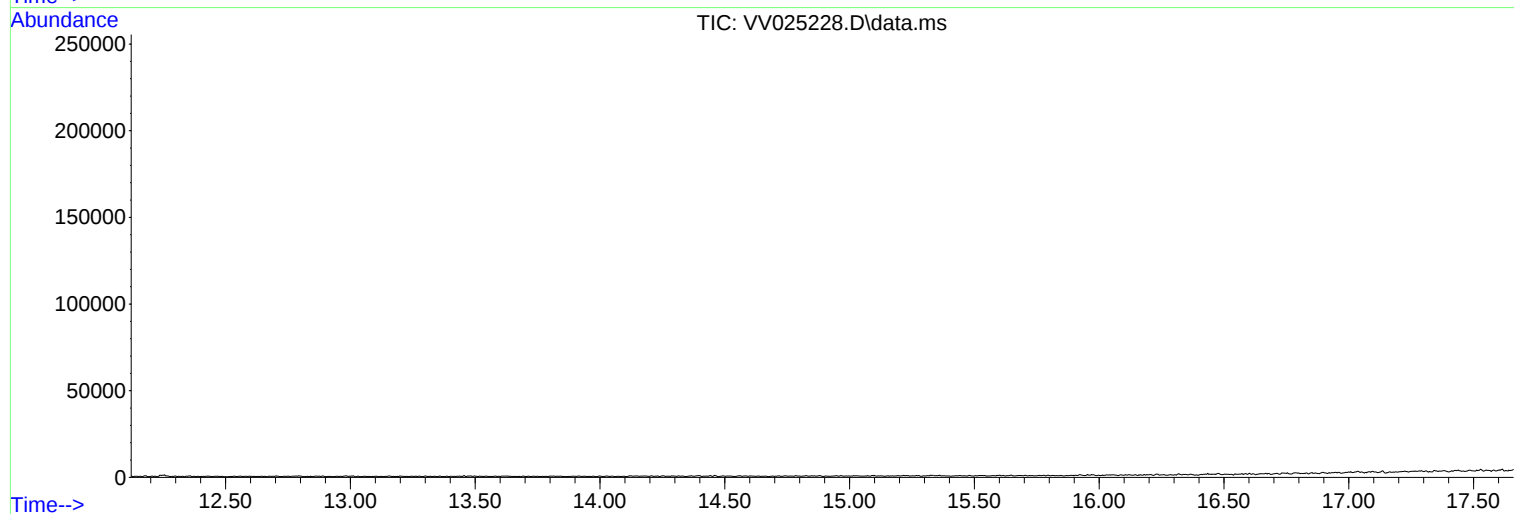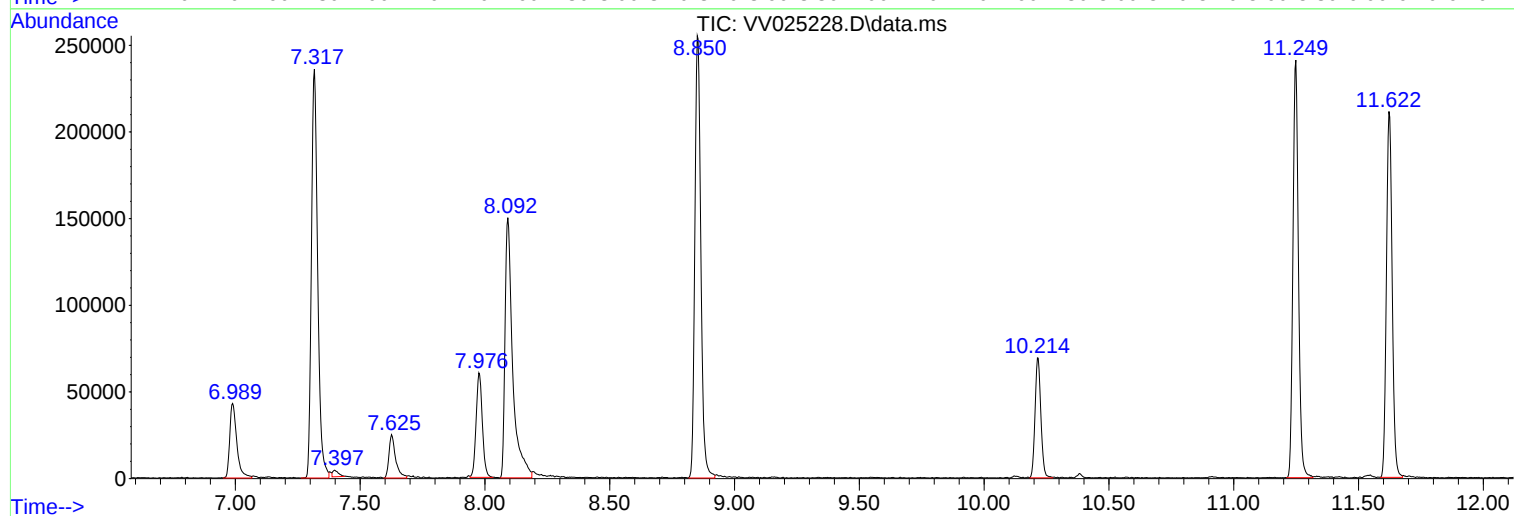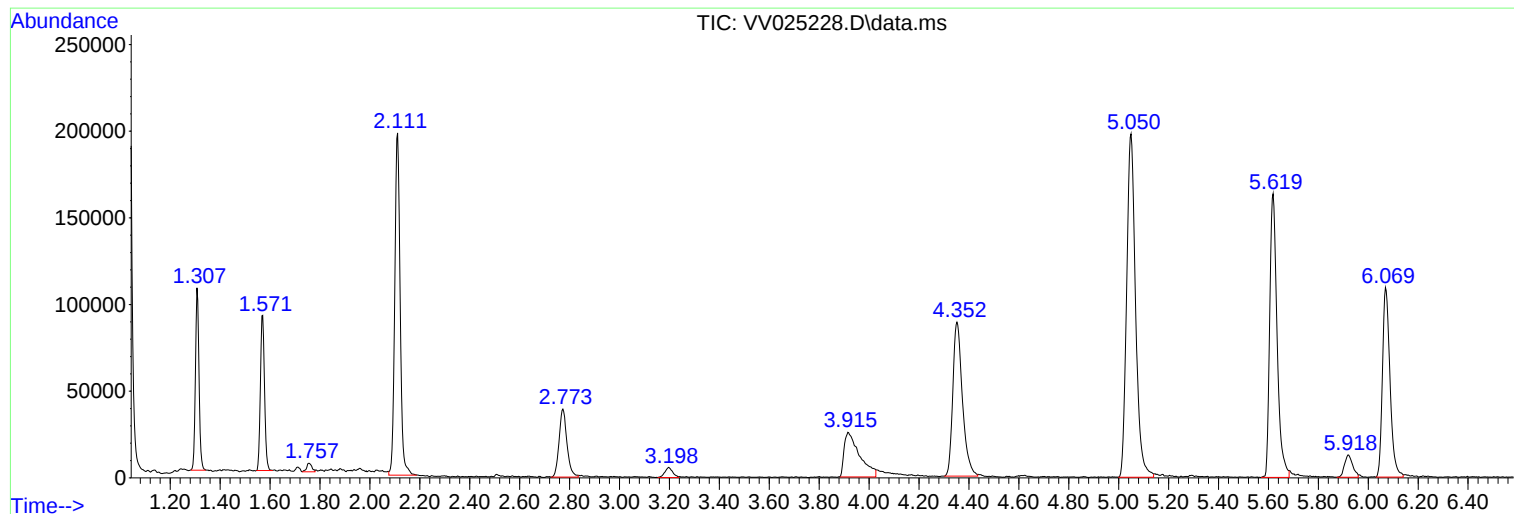

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025228.D
Acq On : 27 Mar 2022 03:21
Operator : SY/MD
Sample : N2097-20
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025228.D
Acq On : 27 Mar 2022 03:21
Operator : SY/MD
Sample : N2097-20
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
