

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
 Data File : VV025232.D
 Acq On : 27 Mar 2022 04:55
 Operator : SY/MD
 Sample : N2110-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0PB4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025232.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	104045	106600	11.87%	2.165%
2	1.571	156	165	176	rBV	90462	105072	11.70%	2.134%
3	2.111	321	333	350	rVB	199381	296499	33.01%	6.022%
4	3.915	884	894	930	rBV2	25119	114406	12.74%	2.324%
5	4.352	1015	1030	1052	rBV	87845	229657	25.57%	4.664%
6	5.050	1230	1247	1280	rBV2	195887	490619	54.63%	9.964%
7	5.619	1411	1424	1455	rBV	159873	335346	37.34%	6.811%
8	5.911	1503	1515	1531	rVB9	4690	10600	1.18%	0.215%
9	6.069	1547	1564	1584	rBV2	108607	228707	25.47%	4.645%
10	6.989	1837	1850	1868	rBV2	44441	83823	9.33%	1.702%
11	7.317	1939	1952	1970	rBV	237986	420827	46.86%	8.547%
12	7.625	2039	2048	2065	rBV	23376	42371	4.72%	0.861%
13	7.972	2144	2156	2173	rBV	533757	898077	100.00%	18.240%
14	8.091	2183	2193	2228	rBV	159086	323649	36.04%	6.573%
15	8.850	2418	2429	2450	rBV	249714	413372	46.03%	8.395%
16	10.214	2841	2853	2865	rBV	69810	111957	12.47%	2.274%
17	11.246	3163	3174	3193	rBV	229109	359060	39.98%	7.292%
18	11.535	3250	3264	3276	rBV5	5363	10491	1.17%	0.213%
19	11.622	3279	3291	3314	rVB	215381	342655	38.15%	6.959%




Sum of corrected areas: 4923788

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025232.D
Acq On : 27 Mar 2022 04:55
Operator : SY/MD
Sample : N2110-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

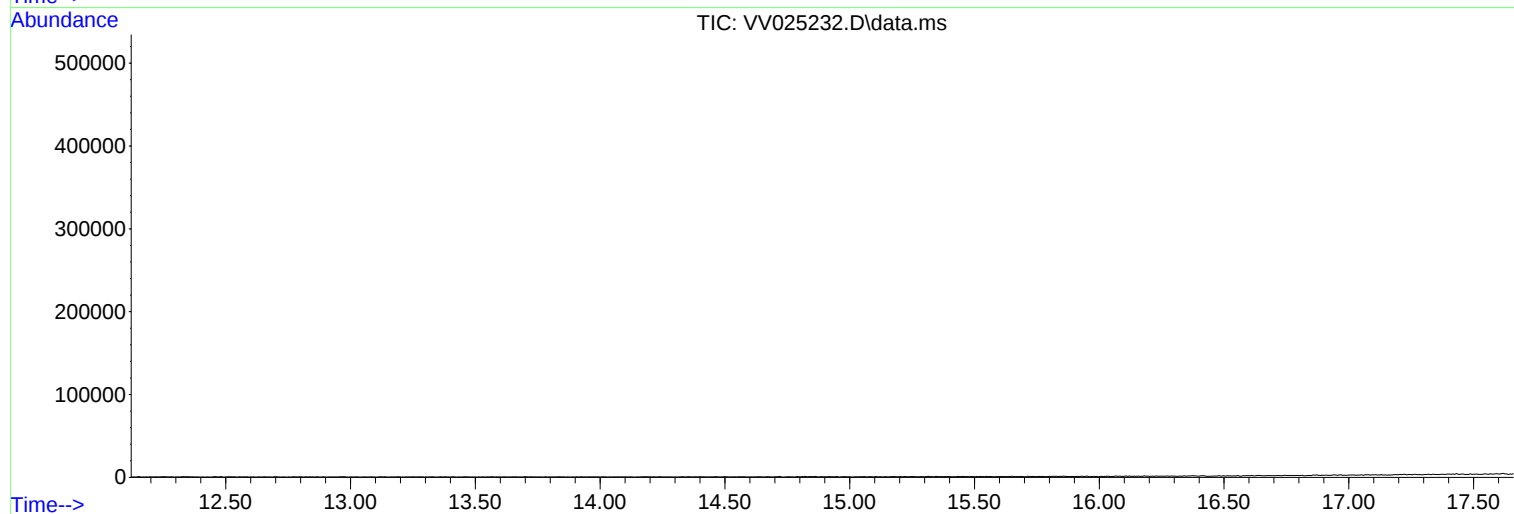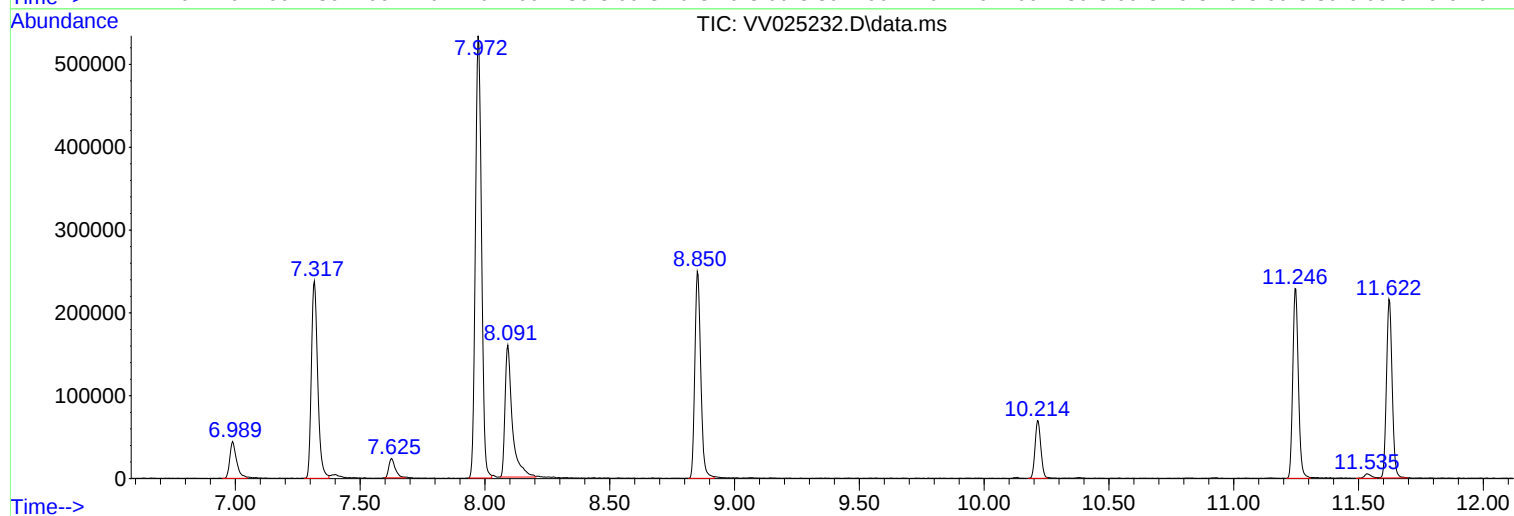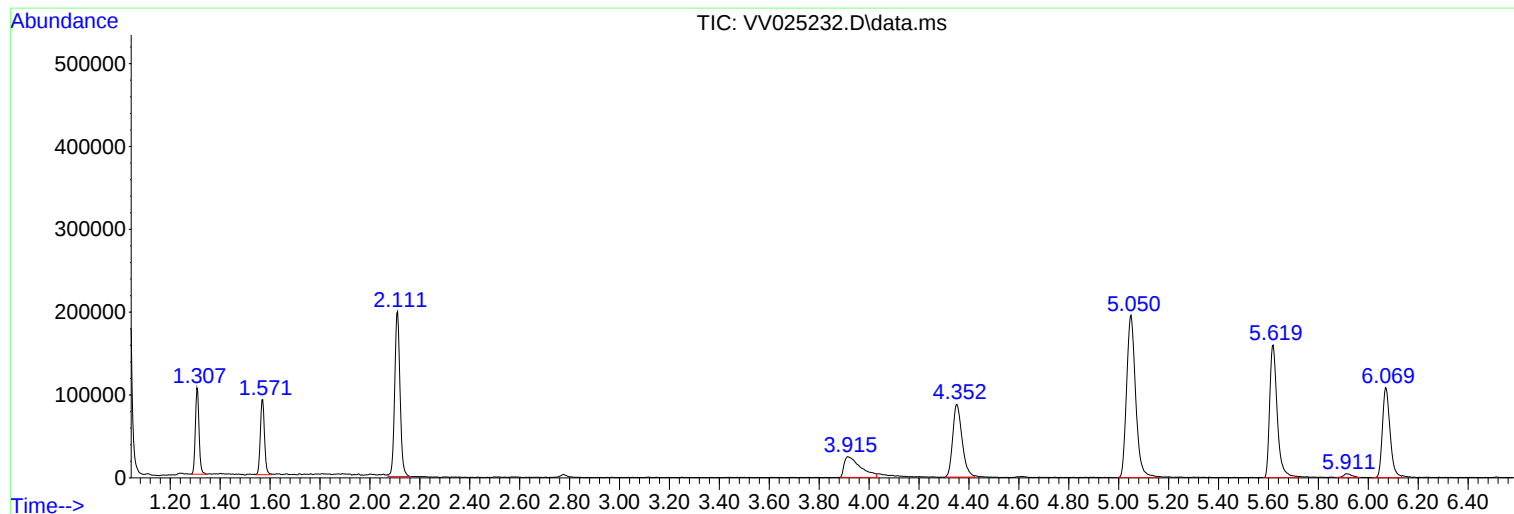

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025232.D
Acq On : 27 Mar 2022 04:55
Operator : SY/MD
Sample : N2110-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025232.D
Acq On : 27 Mar 2022 04:55
Operator : SY/MD
Sample : N2110-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc