

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
 Data File : VV025240.D
 Acq On : 27 Mar 2022 08:02
 Operator : SY/MD
 Sample : N2110-12
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0PC8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025240.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	73	83	96	rVB2	111814	152307	28.35%	3.472%
2	1.391	102	109	117	rBV3	3884	6753	1.26%	0.154%
3	1.571	157	165	177	rVB	90310	99724	18.56%	2.274%
4	2.111	321	333	353	rVB	187521	274866	51.17%	6.267%
5	3.912	882	893	913	rBV2	25917	94866	17.66%	2.163%
6	4.371	1014	1036	1067	rBV4	160250	537197	100.00%	12.247%
7	5.050	1232	1247	1269	rBV2	189680	472625	87.98%	10.775%
8	5.619	1412	1424	1444	rBV	165438	334215	62.21%	7.620%
9	5.911	1506	1515	1527	rVB7	4956	9800	1.82%	0.223%
10	6.069	1552	1564	1589	rBV	106173	220097	40.97%	5.018%
11	6.513	1691	1702	1719	rBV2	20911	44533	8.29%	1.015%
12	6.989	1839	1850	1879	rBV	42795	83939	15.63%	1.914%
13	7.317	1941	1952	1971	rBV	232431	408361	76.02%	9.310%
14	7.625	2039	2048	2069	rBV2	23626	45871	8.54%	1.046%
15	7.976	2147	2157	2174	rVB3	33245	58965	10.98%	1.344%
16	8.091	2183	2193	2222	rBV2	146736	313402	58.34%	7.145%
17	8.850	2418	2429	2453	rBV	253152	421900	78.54%	9.619%
18	10.217	2841	2854	2867	rBV	67445	106869	19.89%	2.436%
19	11.249	3162	3175	3190	rBV	230124	360867	67.18%	8.227%
20	11.532	3256	3263	3277	rBV5	6466	11319	2.11%	0.258%
21	11.622	3280	3291	3311	rVV	208330	327777	61.02%	7.473%




Sum of corrected areas: 4386253

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025240.D
Acq On : 27 Mar 2022 08:02
Operator : SY/MD
Sample : N2110-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PC8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

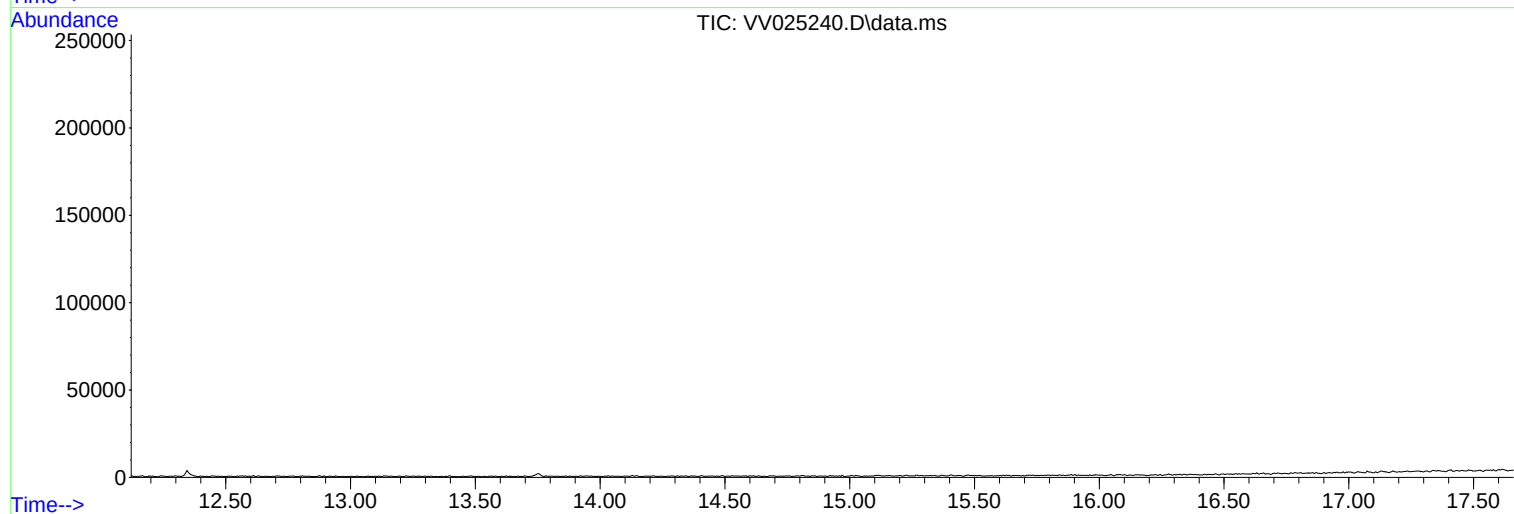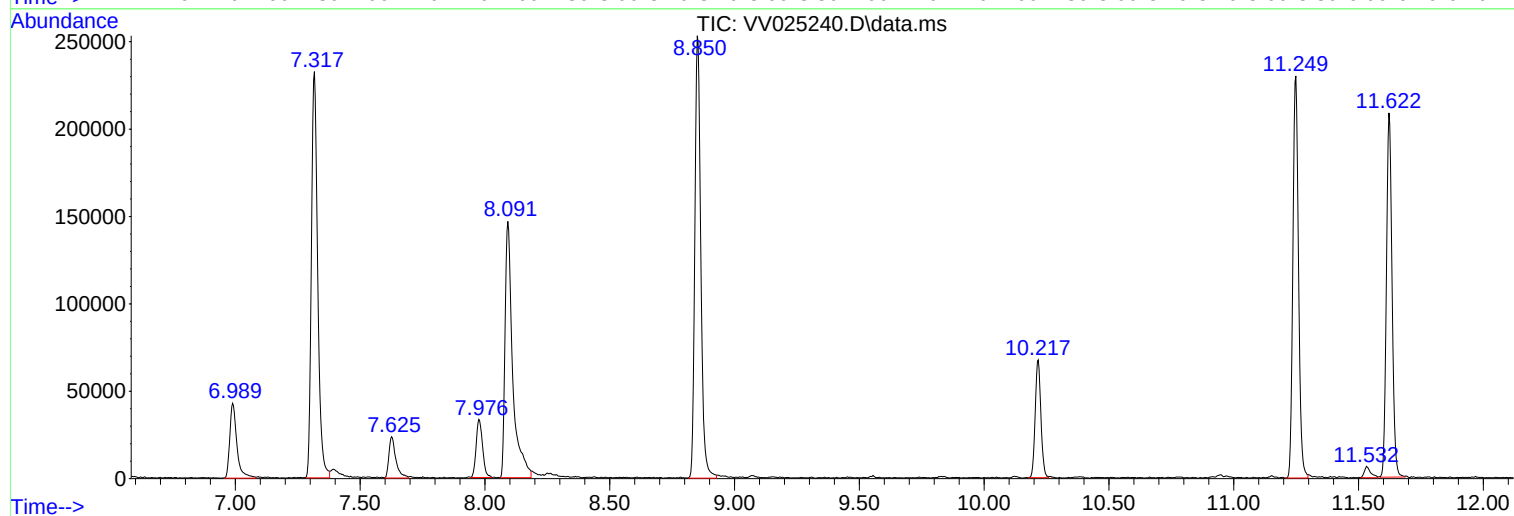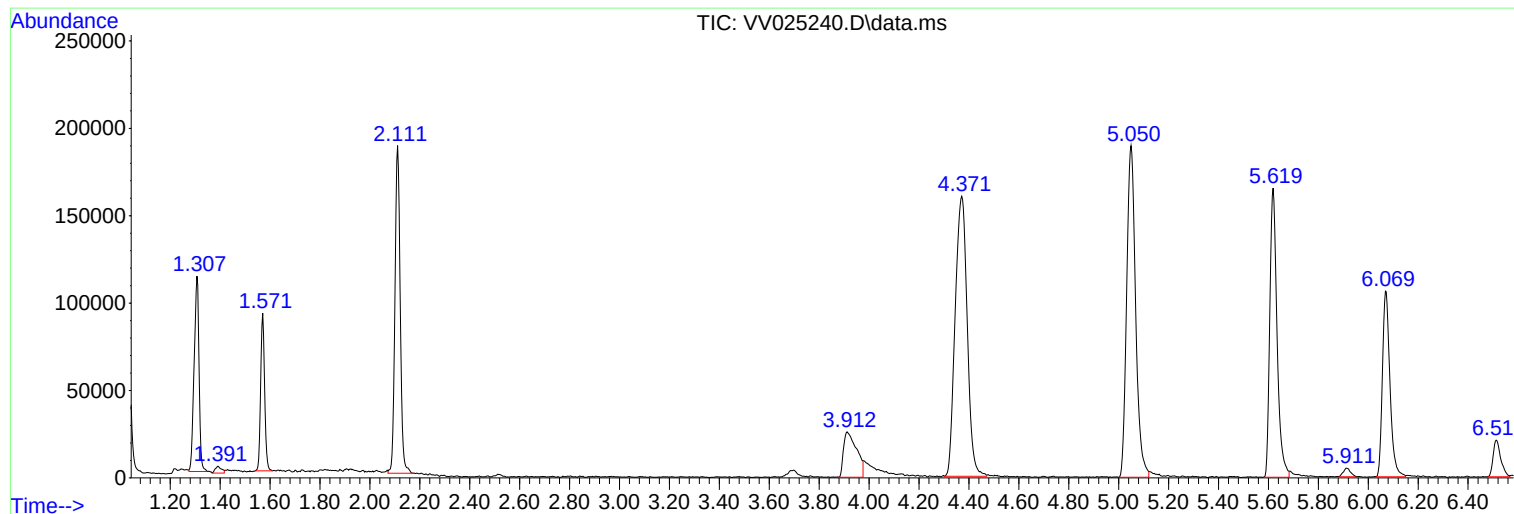

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025240.D
Acq On : 27 Mar 2022 08:02
Operator : SY/MD
Sample : N2110-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PC8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025240.D
Acq On : 27 Mar 2022 08:02
Operator : SY/MD
Sample : N2110-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PC8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc