

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
 Data File : VV025242.D
 Acq On : 27 Mar 2022 08:49
 Operator : SY/MD
 Sample : N2101-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YAYW8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025242.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	50	56	60	rBV3	5026	5464	1.24%	0.141%
2	1.310	77	84	95	rVB	88012	90192	20.46%	2.319%
3	1.571	156	165	177	rBV	81045	92316	20.94%	2.374%
4	2.111	322	333	355	rVB	170664	261650	59.35%	6.728%
5	3.153	647	657	673	rBV2	10190	24103	5.47%	0.620%
6	3.905	877	891	927	rBV2	30084	115131	26.12%	2.960%
7	4.352	1015	1030	1052	rBV2	79058	197231	44.74%	5.072%
8	5.050	1232	1247	1273	rBV2	178027	440846	100.00%	11.336%
9	5.619	1410	1424	1460	rBV	163825	335136	76.02%	8.618%
10	6.069	1552	1564	1587	rBV	100640	209172	47.45%	5.379%
11	6.989	1838	1850	1870	rBV	38400	72646	16.48%	1.868%
12	7.317	1940	1952	1971	rBV	214129	377520	85.64%	9.708%
13	7.625	2038	2048	2067	rBV	21282	38674	8.77%	0.994%
14	7.976	2147	2157	2175	rBV	62881	106870	24.24%	2.748%
15	8.091	2183	2193	2231	rBV	143600	302521	68.62%	7.779%
16	8.776	2396	2406	2415	rBV4	9141	15199	3.45%	0.391%
17	8.850	2418	2429	2457	rBV	247630	415875	94.34%	10.694%
18	10.214	2841	2853	2867	rBV2	69011	109187	24.77%	2.808%
19	11.249	3164	3175	3190	rBV	233794	361458	81.99%	9.294%
20	11.538	3255	3265	3273	rBV5	3457	5987	1.36%	0.154%
21	11.622	3278	3291	3309	rBV	200019	311768	70.72%	8.017%




Sum of corrected areas: 3888946

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025242.D
Acq On : 27 Mar 2022 08:49
Operator : SY/MD
Sample : N2101-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAYW8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

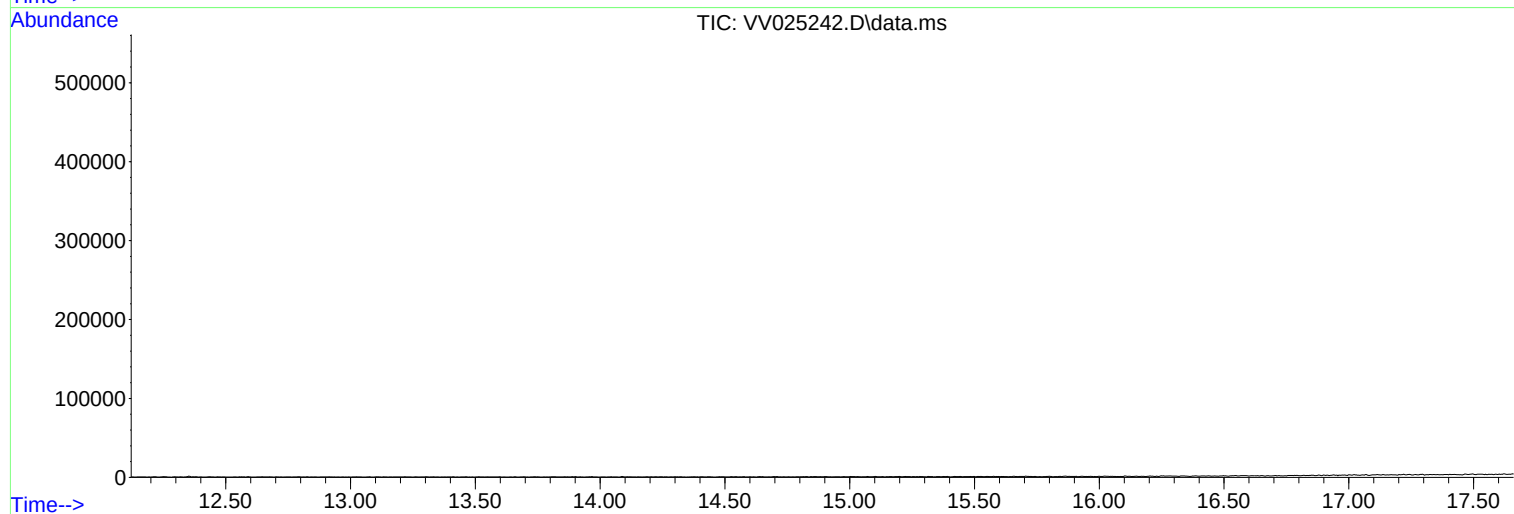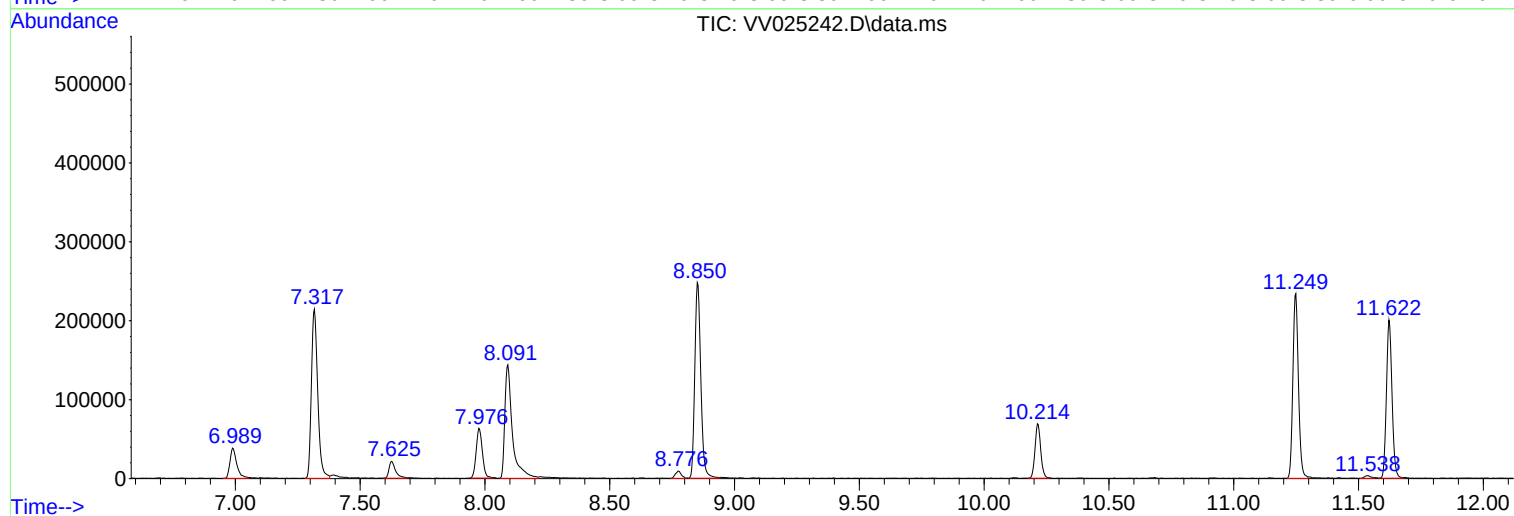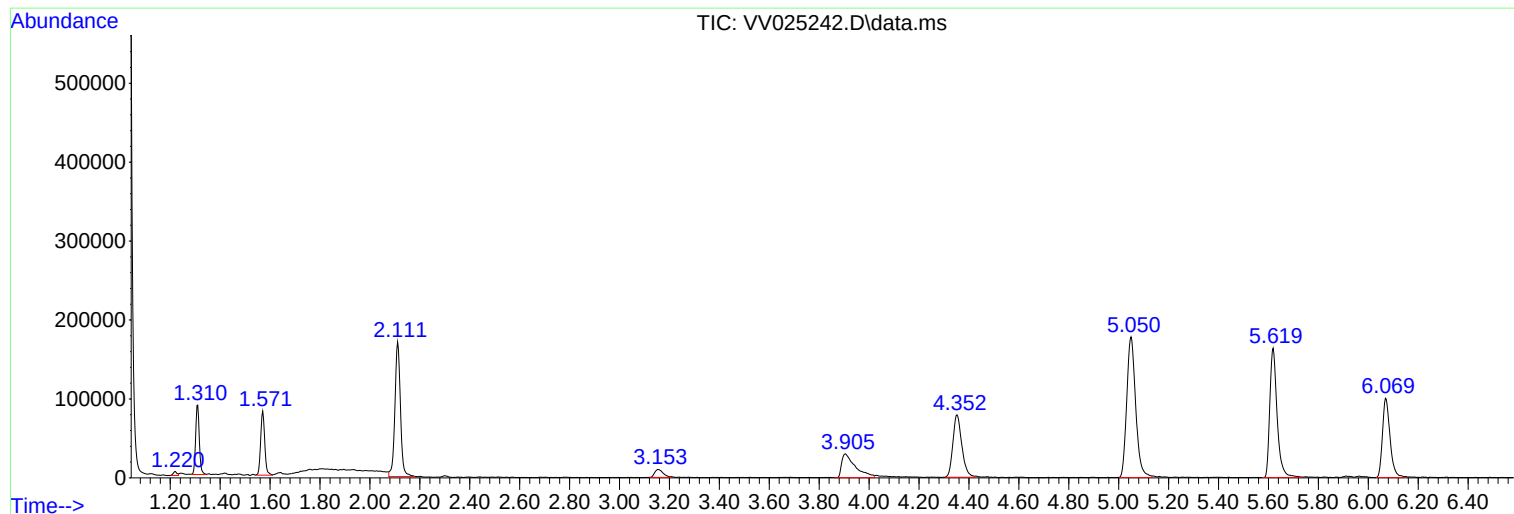

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025242.D
Acq On : 27 Mar 2022 08:49
Operator : SY/MD
Sample : N2101-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAYW8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032622\
Data File : VV025242.D
Acq On : 27 Mar 2022 08:49
Operator : SY/MD
Sample : N2101-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAYW8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
