

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032724\
 Data File : VV034863.D
 Acq On : 27 Mar 2024 14:29
 Operator : SY/MD
 Sample : P1851-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 28 01:55:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 28 01:53:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	337812	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	331691	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	155272	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	104647	32.076	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	64.160%	
7) Chloroethane-d5	1.532	69	100576	35.494	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	70.980%	
11) 1,1-Dichloroethene-d2	2.060	65	48536	33.939	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	67.880%	
21) 2-Butanone-d5	3.786	46	161891	83.670	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	83.670%	
24) Chloroform-d	4.249	84	223348	40.718	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	81.440%	
26) 1,2-Dichloroethane-d4	4.941	65	143976	41.342	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	82.680%	
32) Benzene-d6	4.960	84	417731	37.493	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	74.980%	
36) 1,2-Dichloropropane-d6	5.989	67	143501	40.560	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	81.120%	
41) Toluene-d8	7.243	98	352532	35.134	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	70.260%#	
43) trans-1,3-Dichloroprop...	7.555	79	59826	34.783	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	69.560%	
47) 2-Hexanone-d5	8.024	63	108475	81.093	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	81.090%	
56) 1,1,2,2-Tetrachloroeth...	10.153	84	214132	43.950	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	87.900%	
66) 1,2-Dichlorobenzene-d4	11.561	152	143456	41.150	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	82.300%	
Target Compounds						
61) 1,2,3-Trichloropropane	11.185	75	20539	6.104	ug/L	Qvalue # 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032724\
Data File : VV034863.D
Acq On : 27 Mar 2024 14:29
Operator : SY/MD
Sample : P1851-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Mar 28 01:55:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 28 01:53:40 2024
Response via : Initial Calibration

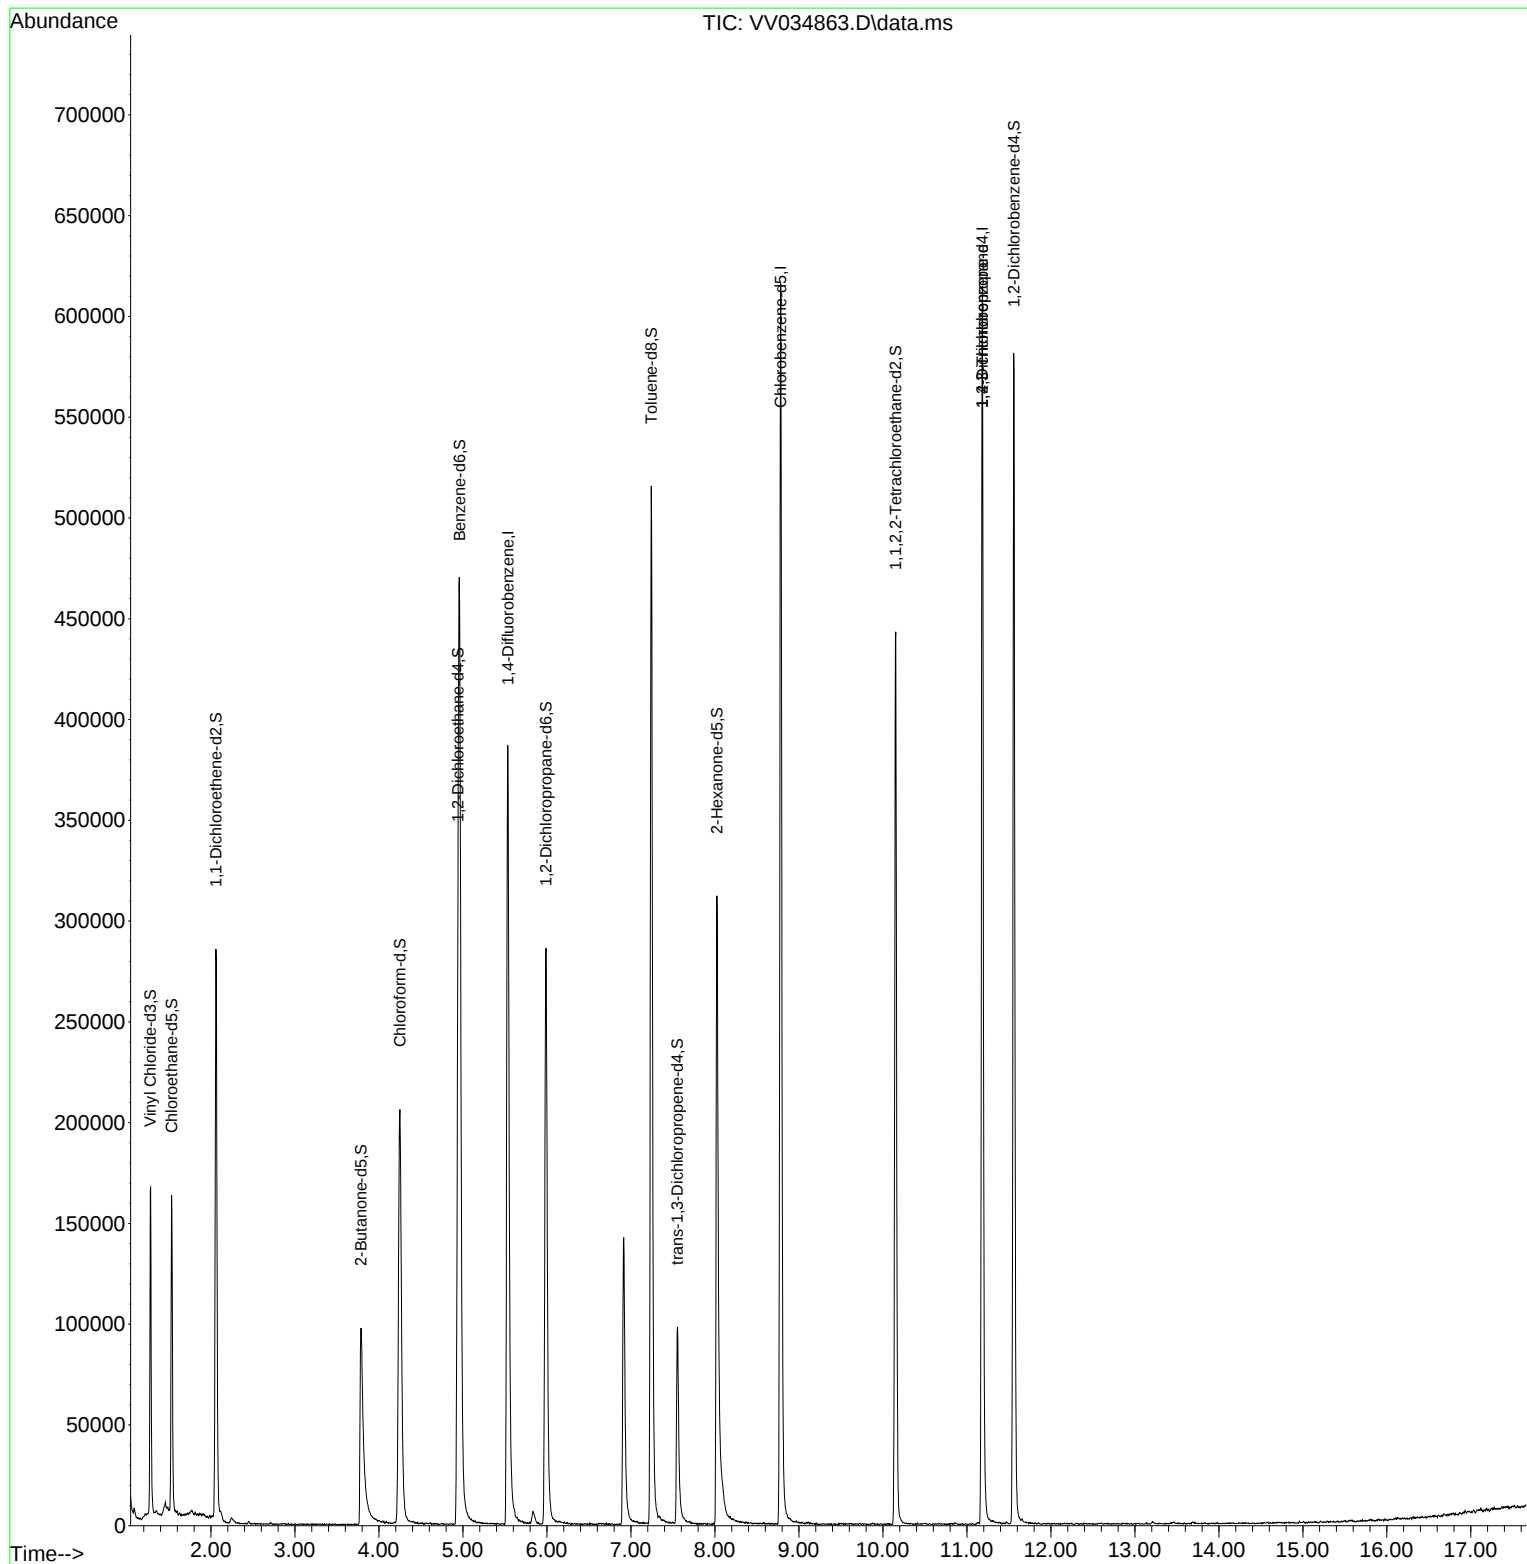

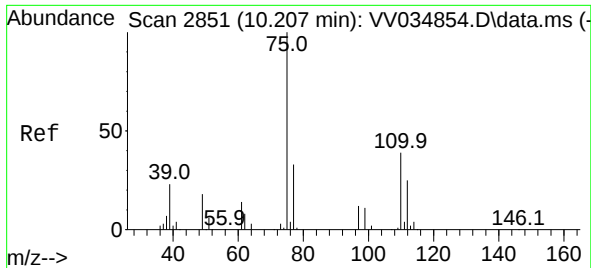

#61
1,2,3-Trichloropropane
Concen: 6.104 ug/L
RT: 11.185 min Scan# 31
Delta R.T. 0.977 min
Lab File: VV034863.D
Acq: 27 Mar 2024 14:29

Instrument :
MSVOA_V
ClientSampleId :

Tgt Ion: 75 Resp: 20539
Ion Ratio Lower Upper
75 100
77 31.0 26.0 39.0
110 2.8 30.5 45.7#

